

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081222\
 Data File : BN021205.D
 Acq On : 13 Aug 2022 10:18
 Operator : CG/JU
 Sample : N4166-01
 Misc :
 ALS Vial : 90 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BGBZ1

Quant Time: Aug 14 23:03:07 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN080322.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Aug 13 04:02:44 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.784	152	3064	0.400	ng/ul	0.00
4) Naphthalene-d8	10.574	136	10112	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.434	164	6704	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.184	188	13375	0.400	ng/ul	0.00
17) Chrysene-d12	21.395	240	9280	0.400	ng/ul	0.00
23) Perylene-d12	23.713	264	9061	0.400	ng/ul	#-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.190	96	17089	4.360	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.186	152	4757	0.321	ng/ul	0.00
18) Fluoranthene-d10	19.221	212	13801	0.482	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.228	88	391	0.097	ng/ul#	58


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081222\
Data File : BN021205.D
Acq On : 13 Aug 2022 10:18
Operator : CG/JU
Sample : N4166-01
Misc :
ALS Vial : 90 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BGBZ1

Quant Time: Aug 14 23:03:07 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN080322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Aug 13 04:02:44 2022
Response via : Initial Calibration

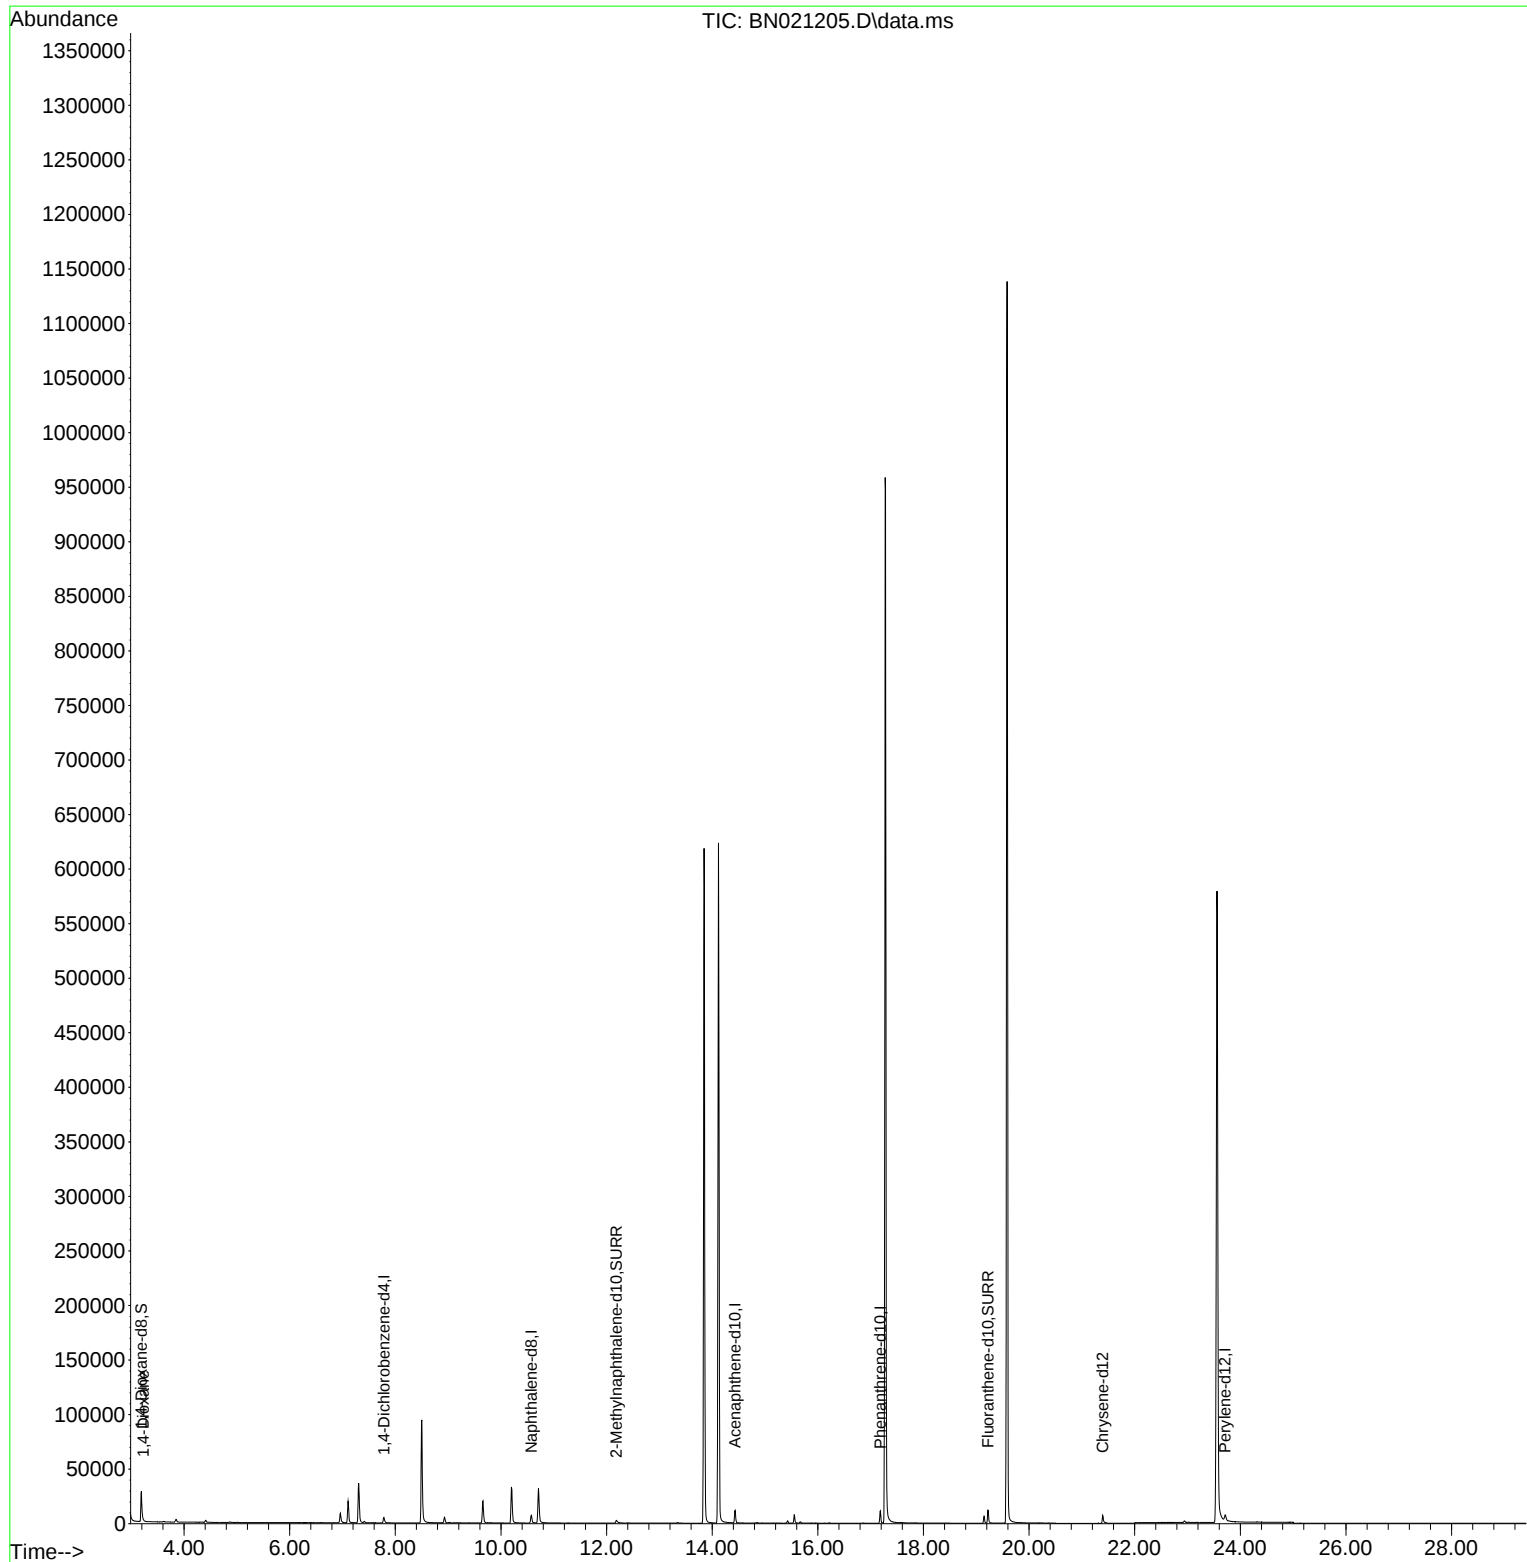

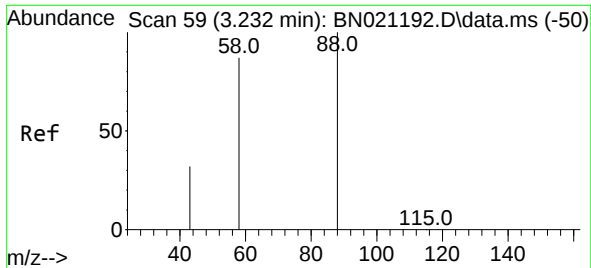

#2
 1,4-Dioxane
 Concen: 0.097 ng/ul
 RT: 3.228 min Scan# 51
 Delta R.T. -0.004 min
 Lab File: BN021205.D
 Acq: 13 Aug 2022 10:18

Instrument :
 BNA_N
 ClientSampleId :
 BGBZ1

Tgt Ion: 88 Resp: 391
 Ion Ratio Lower Upper
 88 100
 43 27.7 31.4 47.0#
 58 18.4 49.0 73.6#

