
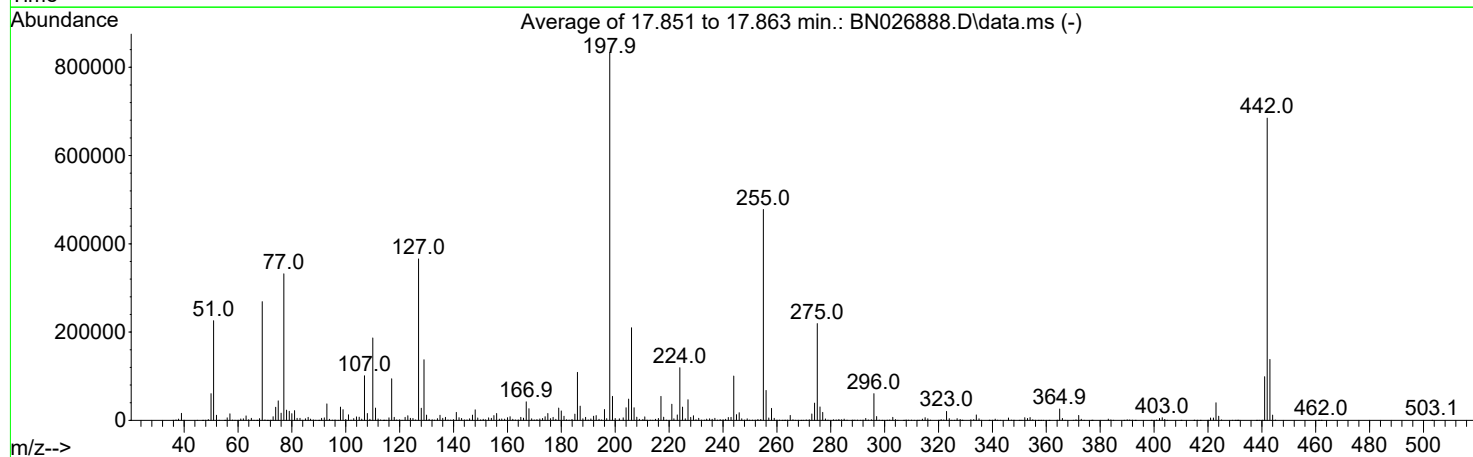


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081223\
Data File : BN026888.D
Acq On : 11 Aug 2023 07:14
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN081123.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Aug 11 01:57:19 2023

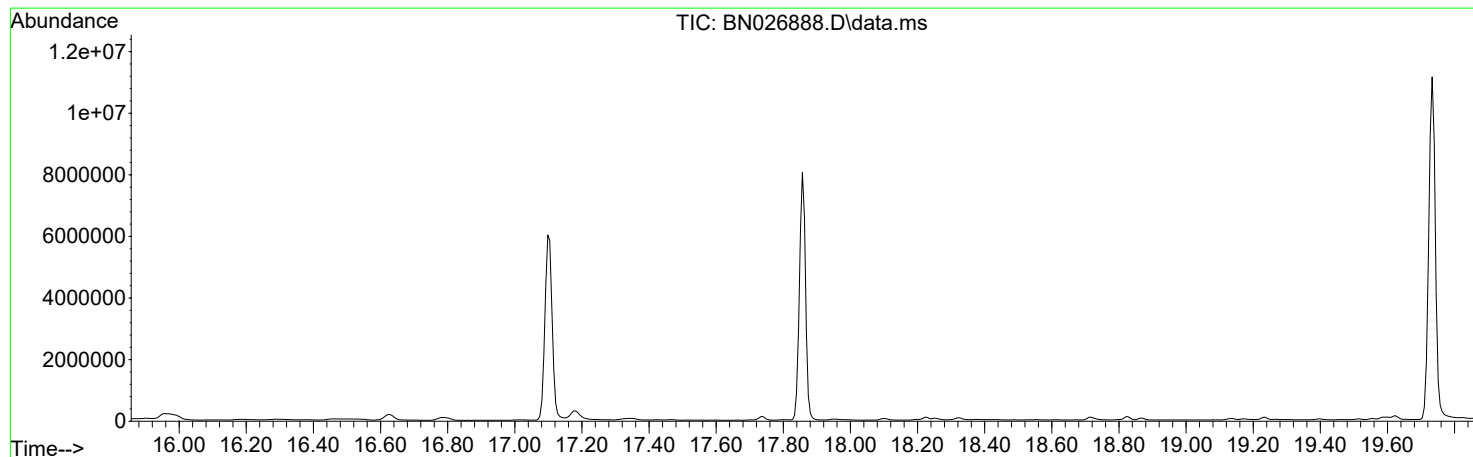




AutoFind: Scans 2544, 2545, 2546; Background Corrected with Scan 2536

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	27.1	225911	PASS
68	69	0.00	2	1.6	4179	PASS
69	198	0.00	100	32.3	269008	PASS
70	69	0.00	2	0.4	1020	PASS
127	198	10	80	43.9	365952	PASS
197	198	0.00	2	0.5	4146	PASS
198	198	100	100	100.0	833472	PASS
199	198	5	9	6.5	54536	PASS
275	198	10	60	26.3	219541	PASS
365	198	1	100	3.1	25885	PASS
441	198	0.01	100	11.9	99131	PASS
442	442	50	100	100.0	684800	PASS
443	442	15	24	20.2	138264	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081223\
Data File : BN026888.D
Acq On : 11 Aug 2023 07:14
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Aug 11 07:44:26 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 11 07:44:22 2023
Response via : Initial Calibration

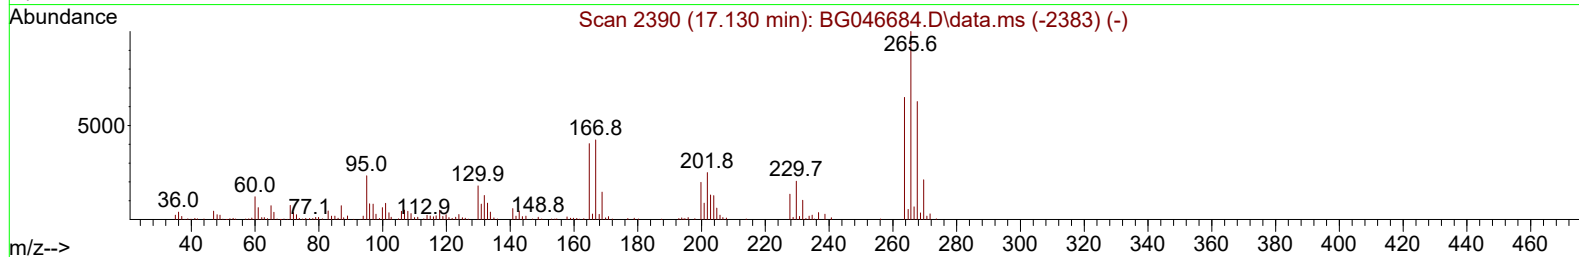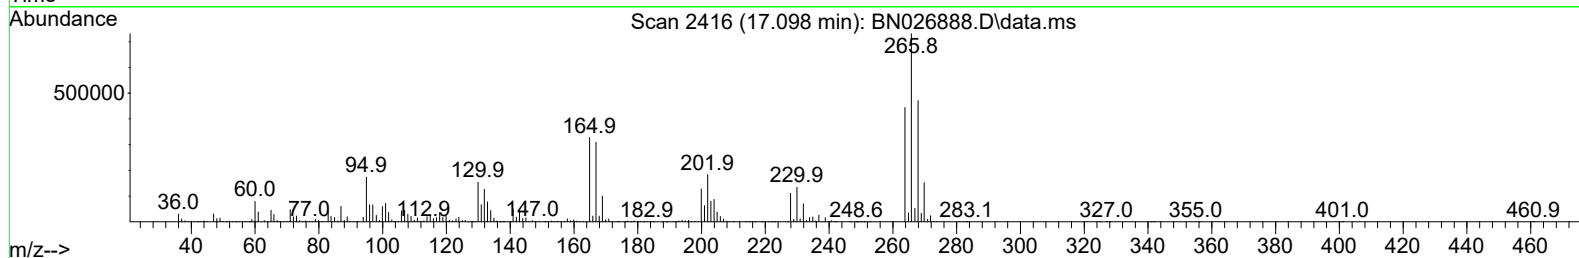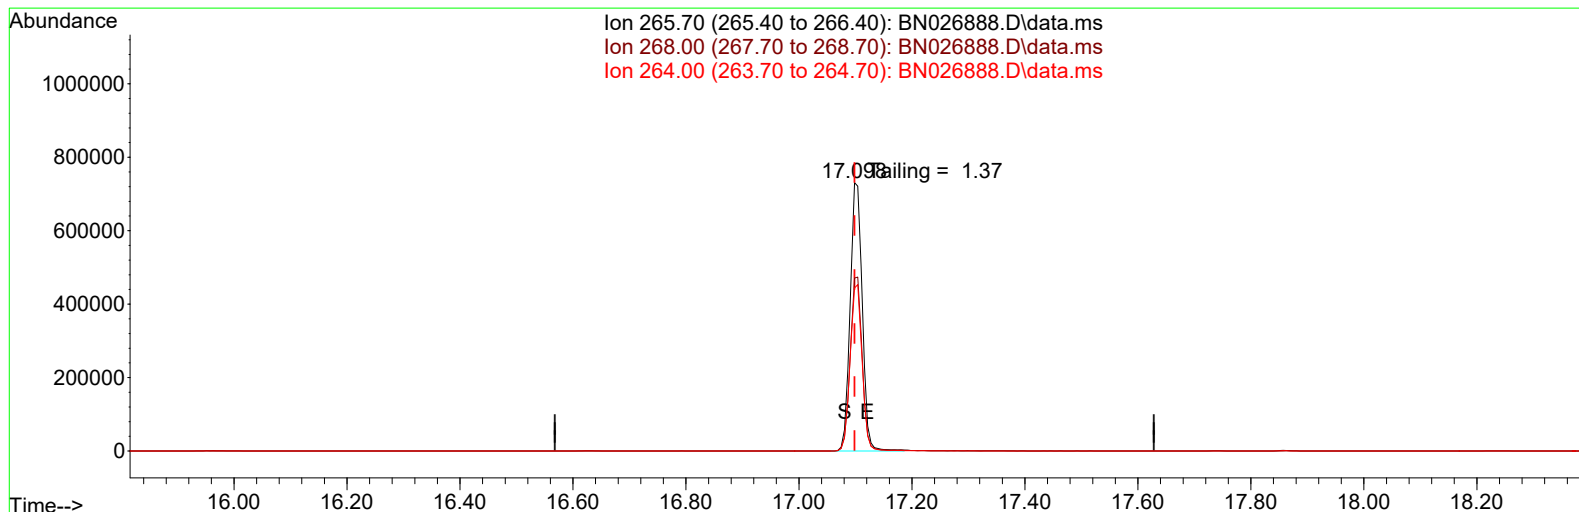

TIC: BN026888.D\data.ms

(70) Pentachlorophenol (C)

17.098min (0.000) 179502.47 ng




response 1095961

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.48
264.00	61.60	60.77
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081223\
Data File : BN026888.D
Acq On : 11 Aug 2023 07:14
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Aug 11 07:44:26 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 11 07:44:22 2023
Response via : Initial Calibration

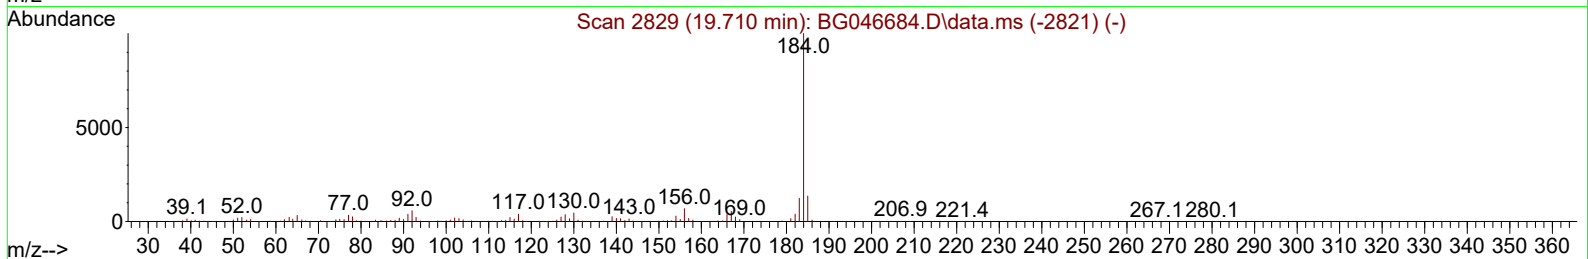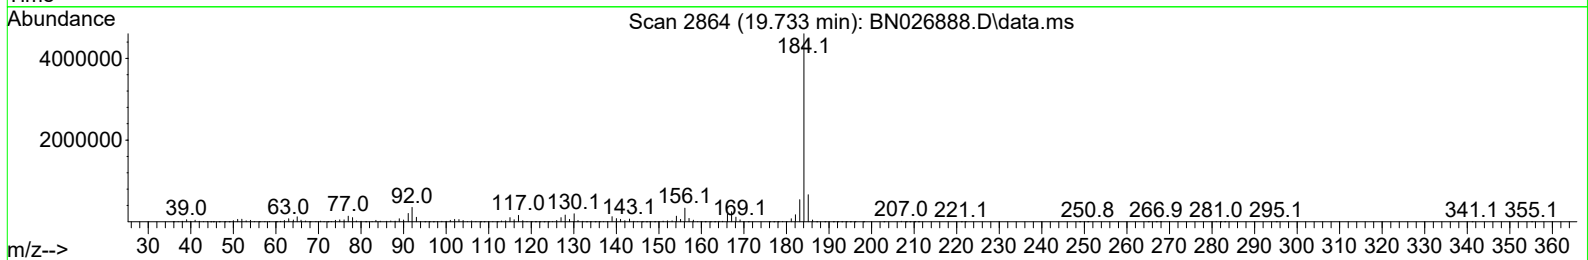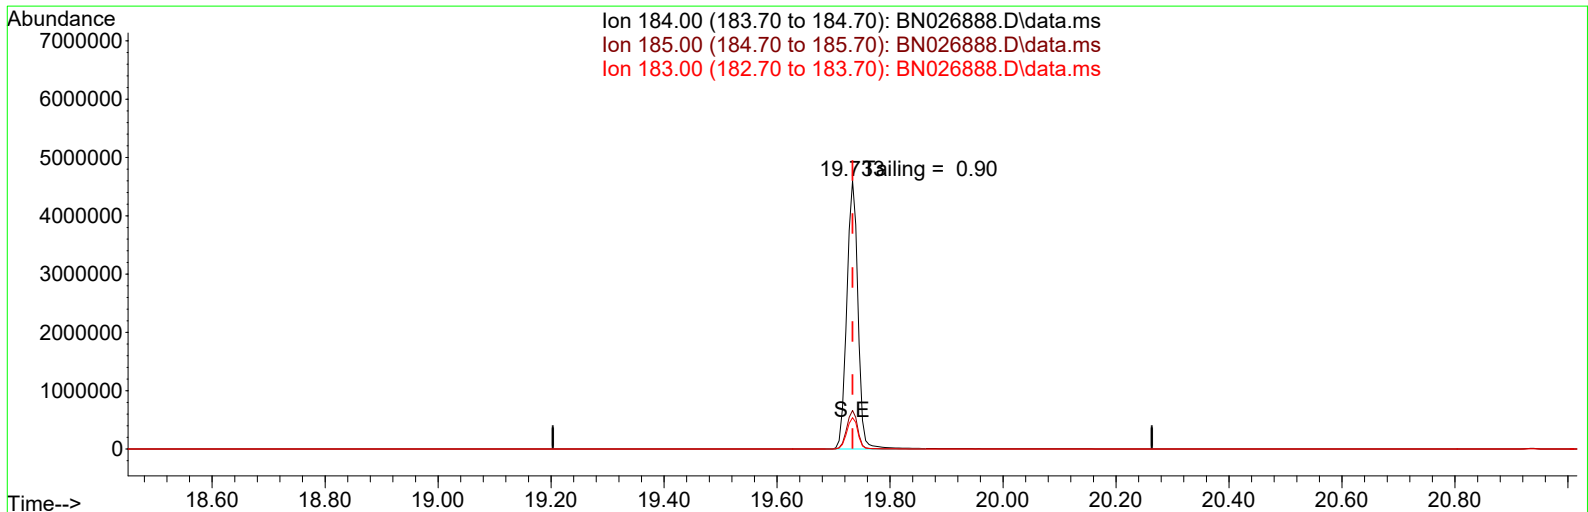

TIC: BN026888.D\data.ms

(77) Benzidine

19.733min (0.000) 4708.87 ng

response 6385697

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.40
183.00	13.20	11.71
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/12/2023	BNA_N	<u>BN026888.D</u>
Compound Name	Response	Retention Time
DDT	2939776	20.939
DDD	34949	20.545
DDE	1074	19.98
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
36023	2975799	1.21

Instrument :
BNA_N
ClientSampleId :
DFTPP