

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN081318\
 Data File : BN002321.D
 Acq On : 14 Aug 2018 00:04
 Operator : JU/SJ
 Sample : J4422-04
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Aug 14 01:23:20 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN081318MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Aug 13 23:38:34 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.68	152	159592	20.00	ng/ul	0.00
18) Naphthalene-d8	10.45	136	763498	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.31	164	472435	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.06	188	1097894	20.00	ng/ul	0.00
77) Chrysene-d12	21.26	240	1227019	20.00	ng/ul	0.00
85) Perylene-d12	23.47	264	1309245	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.24	96	20106	5.95	ng/uL	0.00
5) Phenol-d5	6.86	99	126713	8.66	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.02	67	371665	40.44	ng/ul	0.00
9) 2-Chlorophenol-d4	7.22	132	365416	32.78	ng/ul	0.00
13) 4-Methylphenol-d8	8.38	113	247476	21.15	ng/ul	0.00
19) Nitrobenzene-d5	8.83	128	250101	41.15	ng/ul	0.00
22) 2-Nitrophenol-d4	9.55	143	268126	41.95	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.08	165	420276	35.79	ng/ul	0.00
29) 4-Chloroaniline-d4	10.62	131	4743	0.37	ng/ul	0.03
43) Dimethylphthalate-d6	13.72	166	1687906	43.10	ng/ul	0.00
46) Acenaphthylene-d8	14.00	160	2061832	42.92	ng/ul	0.00
51) 4-Nitrophenol-d4	14.53	143	52844	7.14	ng/ul	0.00
57) Fluorene-d10	15.30	176	1435132	42.27	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.43	200	268559	38.42	ng/ul	0.00
70) Anthracene-d10	17.16	188	2305764	43.96	ng/ul	0.00
78) Pyrene-d10	19.46	212	2650353	45.14	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.34	264	2890782	42.23	ng/ul	0.00


Target Compounds				Ovalue	
45) 2,6-Dinitrotoluene	13.73	165	10541	1.358	ng/ul# 38


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN081318\
Data File : BN002321.D
Acq On : 14 Aug 2018 00:04
Operator : JU/SJ
Sample : J4422-04
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Aug 14 01:23:20 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN081318MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Aug 13 23:38:34 2018
Response via : Initial Calibration

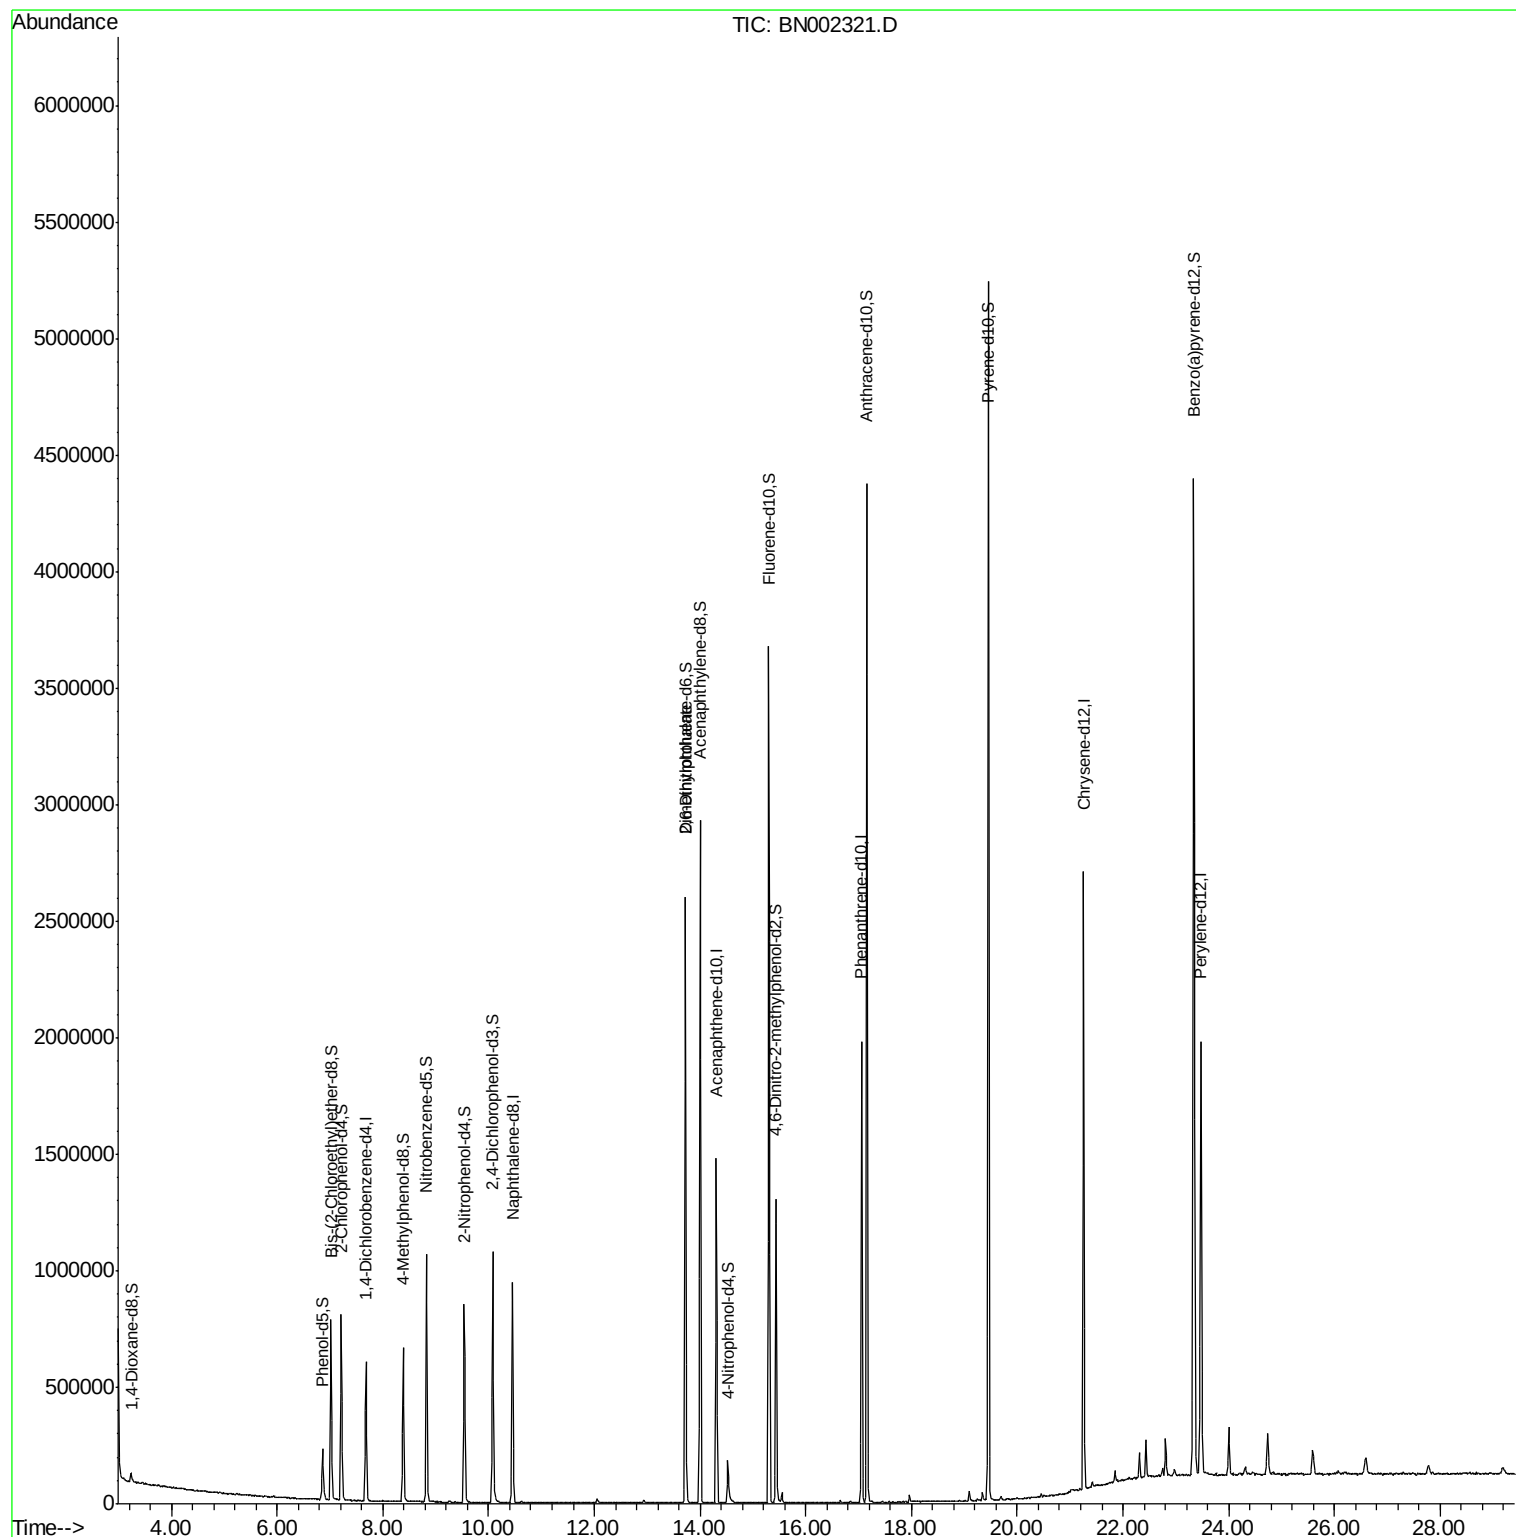

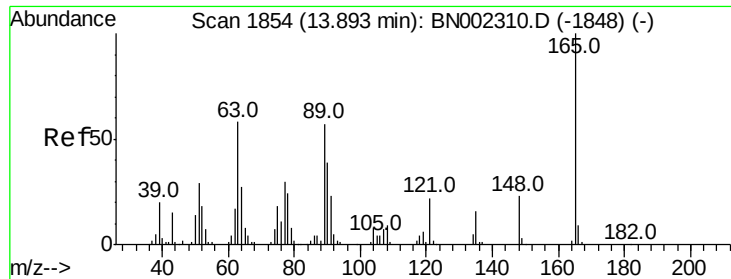

#45

2,6-Dinitrotoluene

Concen: 1.358 ng/ul

RT: 13.73 min Scan# 1826

Delta R.T. -0.16 min

Lab File: BN002321.D

Acq: 14 Aug 2018 00:04

Instrument :

BNA_N

ClientSampleId :



Tot Ion:165 Resp: 10541

Ion Ratio Lower Upper

165 100

89 0.0 42.4 63.6#

121 34.9 16.6 24.8#

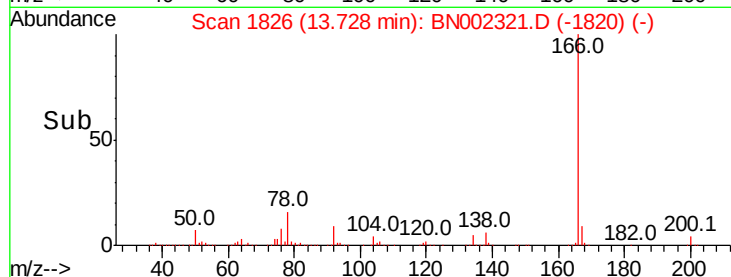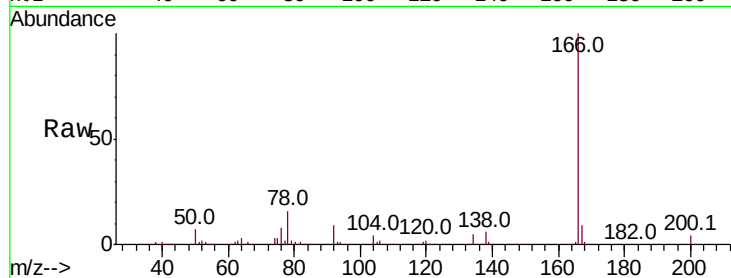

Abundance Ion 165.00 (164.70 to 165.70): E

10000 Ion 89.00 (88.70 to 89.70): BNC

Ion 121.00 (120.70 to 121.70): E

