

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN081319\
 Data File : BN007143.D
 Acq On : 13 Aug 2019 21:55
 Operator : HP/JU
 Sample : PB122017BL
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Aug 14 03:14:32 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-SIM-BN081019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Aug 13 12:12:02 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.43	152	10101	0.40	ng	0.00
6) Naphthalene-d8	10.19	136	39465	0.40	ng	0.00
12) Acenaphthene-d10	14.08	164	22040	0.40	ng	0.00
18) Phenanthrene-d10	16.82	188	50034	0.40	ng	0.00
26) Chrysene-d12	21.05	240	48198	0.40	ng	-0.01
32) Perylene-d12	23.16	264	53495	0.40	ng	-0.01
System Monitoring Compounds						
3) 2-Fluorophenol	5.06	112	8915	0.37	ng	0.00
4) Phenol-d6	6.62	99	11934	0.40	ng	0.00
7) Nitrobenzene-d5	8.56	82	9379	0.29	ng	0.00
10) 2-Methylnaphthalene-d10	11.79	152	21542	0.29	ng	0.00
13) 2,4,6-Tribromophenol	15.57	330	2340	0.20	ng	0.00
14) 2-Fluorobiphenyl	12.71	172	5624	0.18	ng	0.00
24) Fluoranthene-d10	18.87	212	51174	0.29	ng	0.00
28) Terphenyl-d14	19.49	244	40034	0.30	ng	-0.01
Target Compounds						
2) n-Nitrosodimethylamine	3.34	42	155	0.023	ng	# 1
15) Acenaphthylene	13.79	152	12546	0.109	ng	98
17) Fluorene	15.14	166	2229	0.020	ng	# 12

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN081319\
Data File : BN007143.D
Acq On : 13 Aug 2019 21:55
Operator : HP/JU
Sample : PB122017BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Aug 14 03:14:32 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-SIM-BN081019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 13 12:12:02 2019
Response via : Initial Calibration

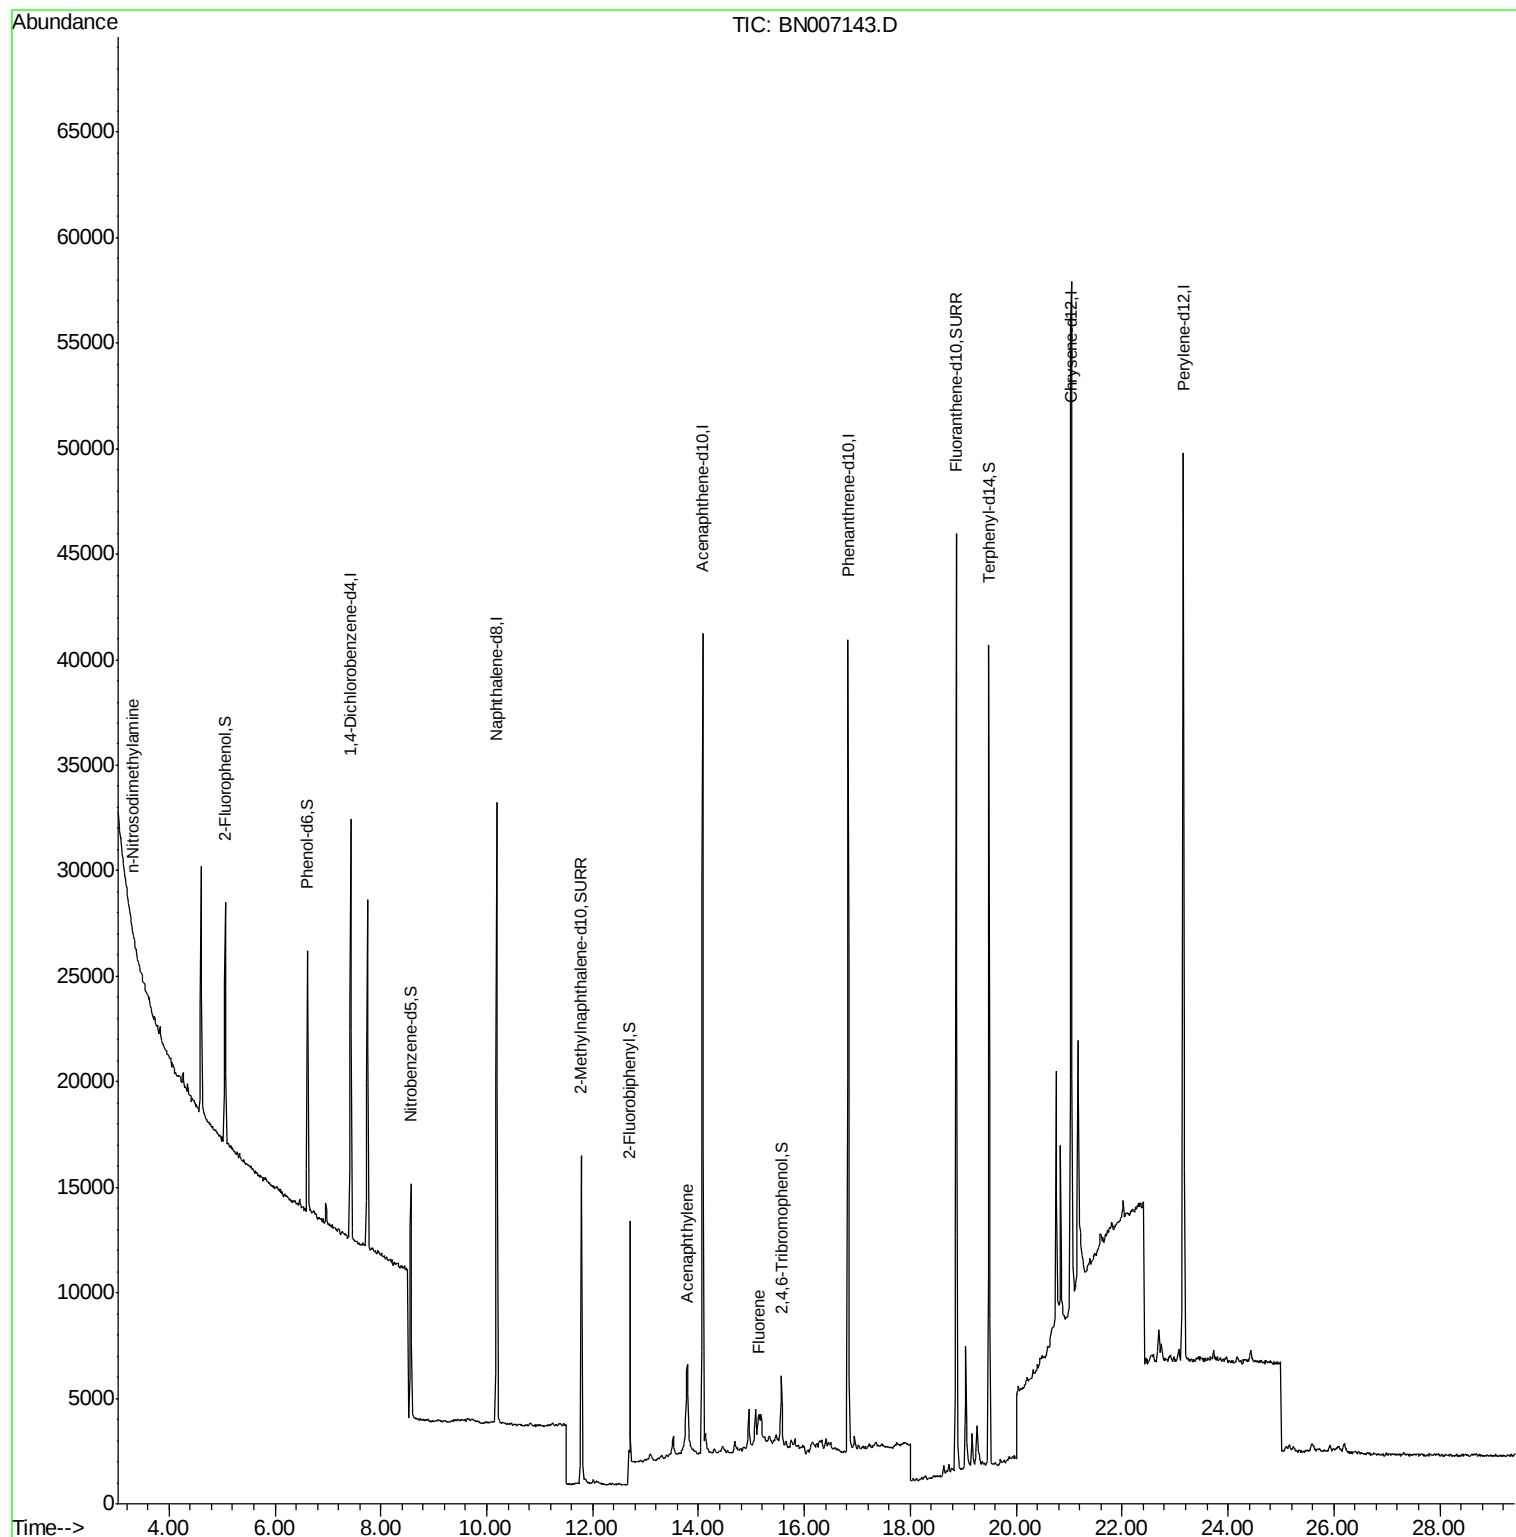




#1




1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 7.43 min Scan# 546
Delta R.T. -0.01 min
Lab File: BN007143.D
Acq: 13 Aug 2019 21:55

Instrument :
BNA_N
ClientSampleId :

Tot Ion:152 Resp: 10101
Ion Ratio Lower Upper
152 100
150 159.7 121.7 182.5
115 61.6 46.2 69.4

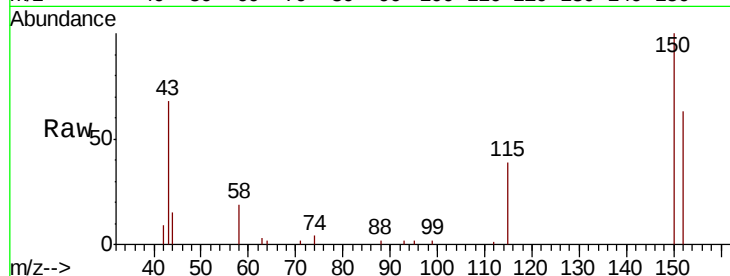


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

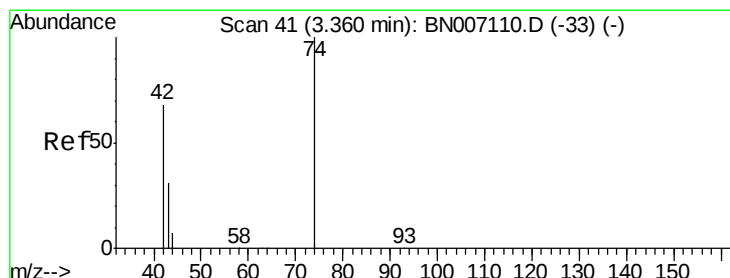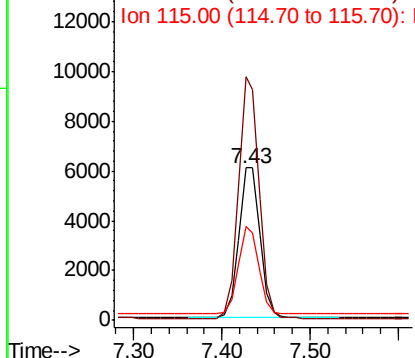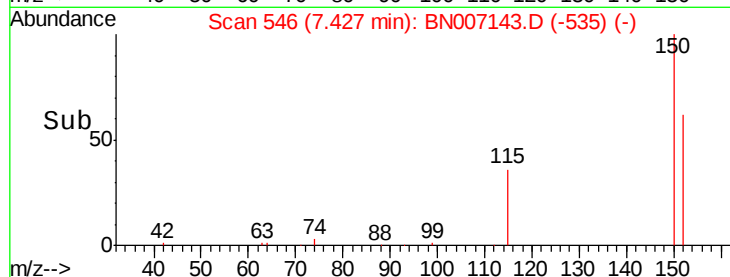



#2


n-Nitrosodimethylamine
Concen: 0.023 ng
RT: 3.34 min Scan# 38
Delta R.T. -0.02 min
Lab File: BN007143.D
Acq: 13 Aug 2019 21:55

Tgt Ion: 42 Resp: 155
Ion Ratio Lower Upper
42 100
74 5.2 110.6 166.0#
44 0.0 0.0 0.0

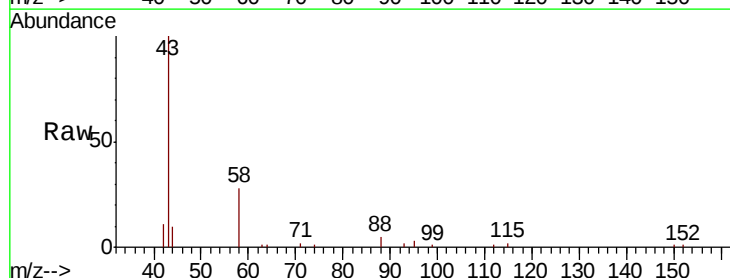

Abundance Ion 42.00 (41.70 to 42.70): BNC
Ion 74.00 (73.70 to 74.70): BNC
Ion 44.00 (43.70 to 44.70): BNC

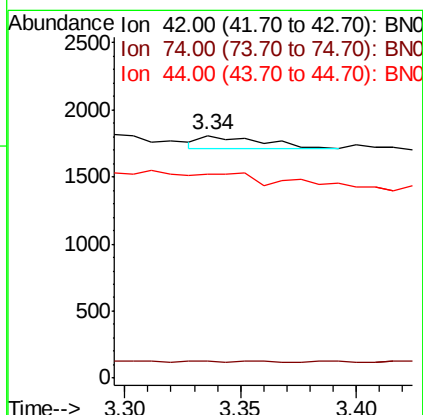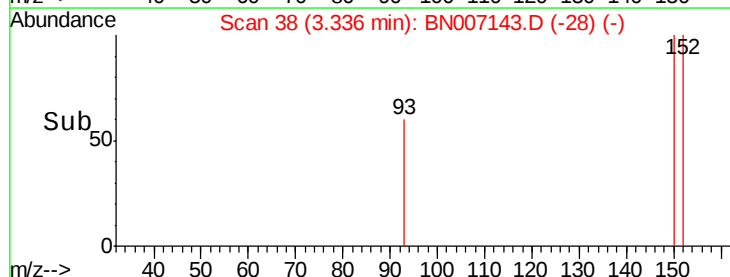

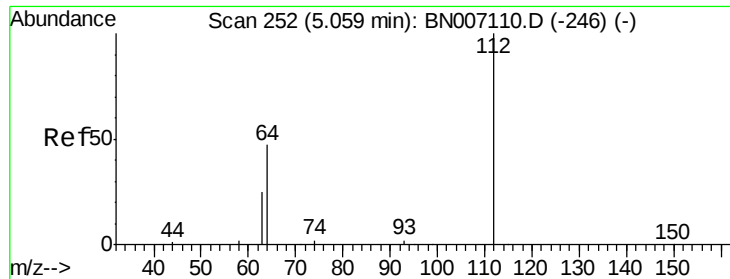

#3

2-Fluorophenol

Concen: 0.367 ng

RT: 5.06 min Scan# 252

Delta R.T. -0.00 min

Lab File: BN007143.D

Acq: 13 Aug 2019 21:55

Instrument :

BNA_N

ClientSampled :


Tot Ion: 112 Resp: 8915

Ion Ratio Lower Upper

112 100

64 51.7 42.6 63.8




63 28.3 22.2 33.2

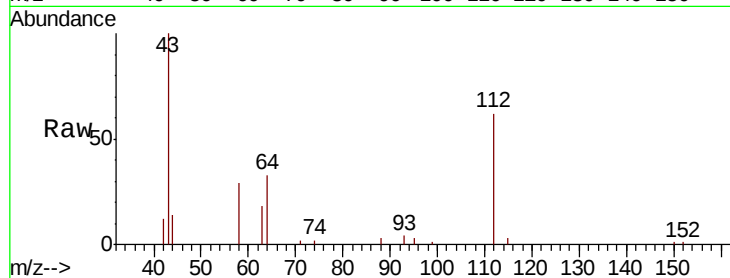

Abundance Ion 112.00 (111.70 to 112.70): BNC

Ion 64.00 (63.70 to 64.70): BNC

Ion 63.00 (62.70 to 63.70): BNC

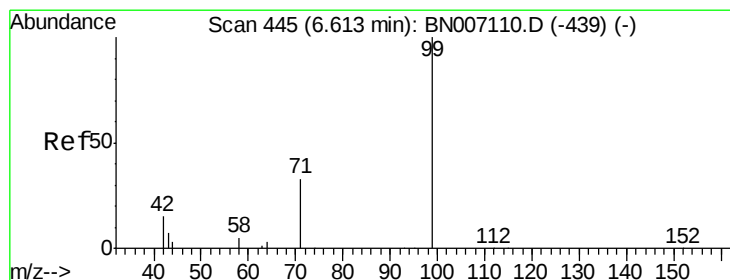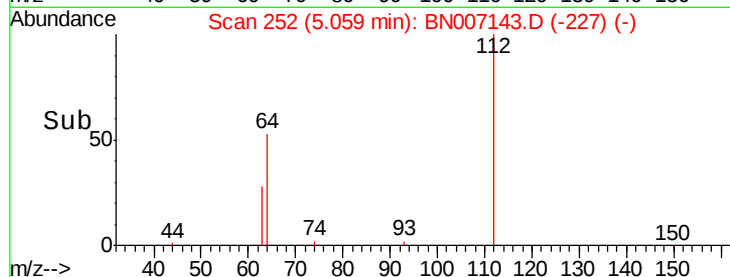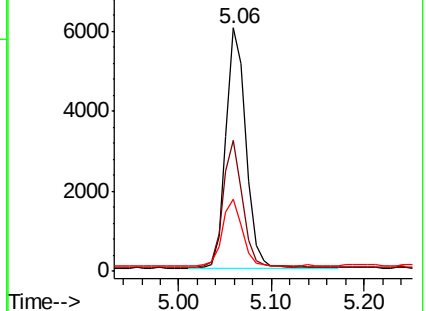

#4

Phenol-d6

Concen: 0.397 ng

RT: 6.62 min Scan# 446

Delta R.T. 0.01 min

Lab File: BN007143.D

Acq: 13 Aug 2019 21:55


Tgt Ion: 99 Resp: 11934

Ion Ratio Lower Upper

99 100

42 17.4 15.8 23.6



71 33.4 27.0 40.4

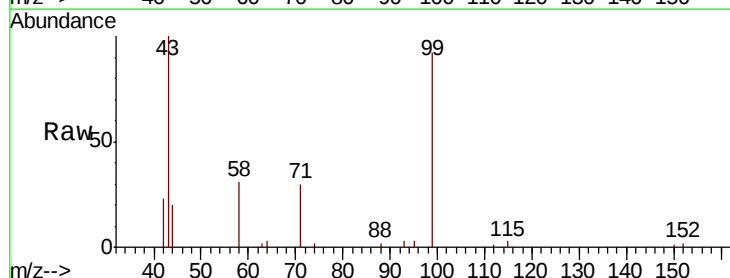


Abundance Ion 99.00 (98.70 to 99.70): BNC

Ion 42.00 (41.70 to 42.70): BNC

Ion 71.00 (70.70 to 71.70): BNC

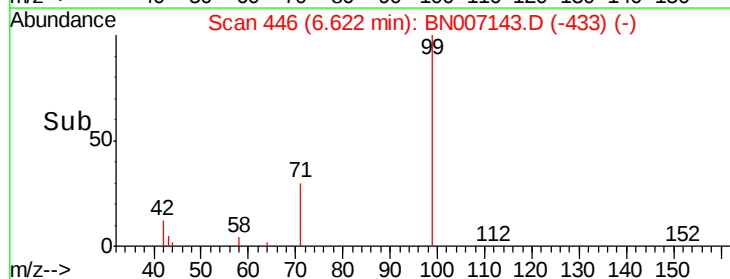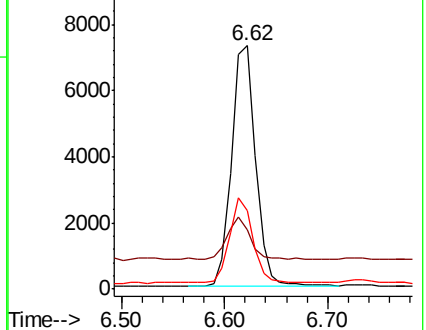

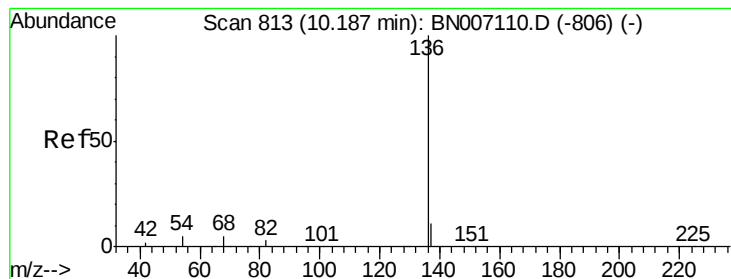

#6

Naphthalene-d8

Concen: 0.400 ng

RT: 10.19 min Scan# 813

Delta R.T. -0.00 min

Lab File: BN007143.D

Acq: 13 Aug 2019 21:55

Instrument :

BNA_N

ClientSampleId :

Tot Ion:136 Resp: 39465


Ion Ratio Lower Upper

136 100

137 11.3 9.4 14.0

54 6.0 6.6 9.8#

68 5.6 6.0 9.0#






Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BNC

Ion 68.00 (67.70 to 68.70): BNC

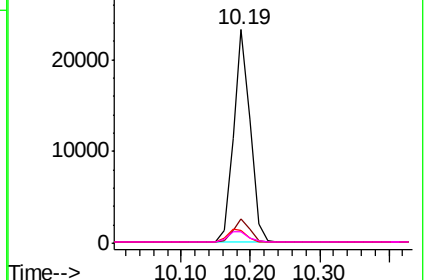

#7

Nitrobenzene-d5

Concen: 0.295 ng

RT: 8.56 min Scan# 685

Delta R.T. -0.00 min

Lab File: BN007143.D

Acq: 13 Aug 2019 21:55


Tgt Ion: 82 Resp: 9379

Ion Ratio Lower Upper

82 100

128 50.3 34.6 51.8



54 41.5 36.2 54.4




Abundance Ion 82.00 (81.70 to 82.70): BNC

Ion 128.00 (127.70 to 128.70): E

Ion 54.00 (53.70 to 54.70): BNC



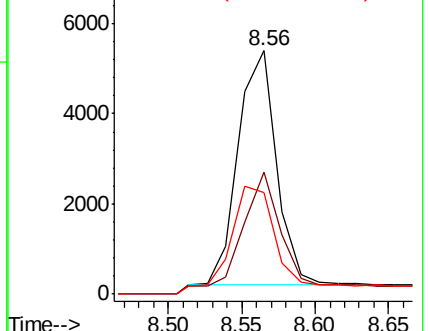





#10
2-Methylnaphthalene-d10
Concen: 0.293 ng
RT: 11.79 min Scan# 981
Delta R.T. -0.00 min
Lab File: BN007143.D
Acq: 13 Aug 2019 21:55




Instrument :
BNA_N
ClientSampleId :


Tot Ion:152 Resp: 21542
Ion Ratio Lower Upper
152 100
151 19.4 15.5 23.3

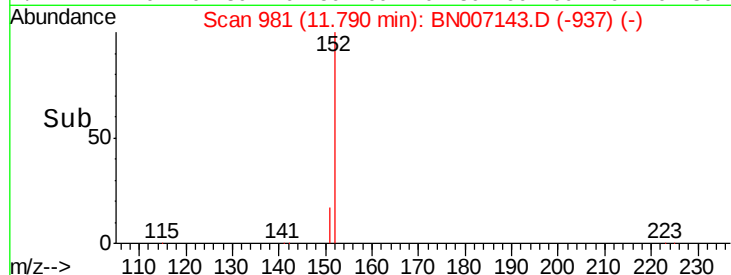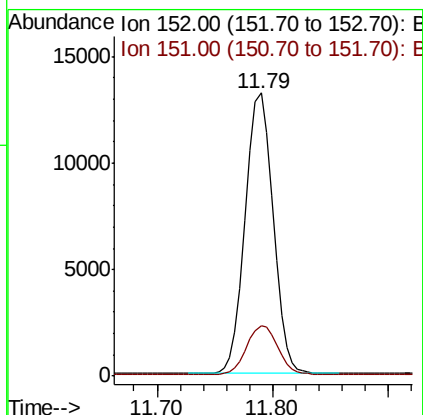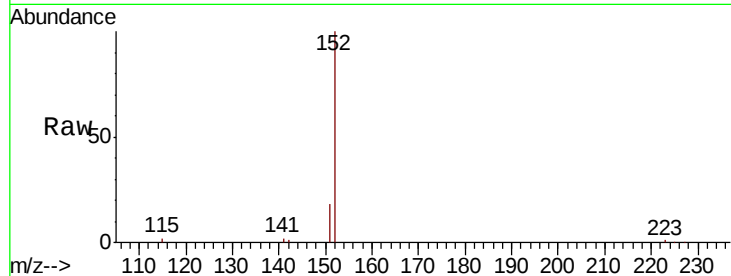

#12
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.08 min Scan# 1310
Delta R.T. -0.00 min
Lab File: BN007143.D
Acq: 13 Aug 2019 21:55

Tgt Ion:164 Resp: 22040
Ion Ratio Lower Upper
164 100
162 101.6 82.2 123.4
160 45.8 38.3 57.5

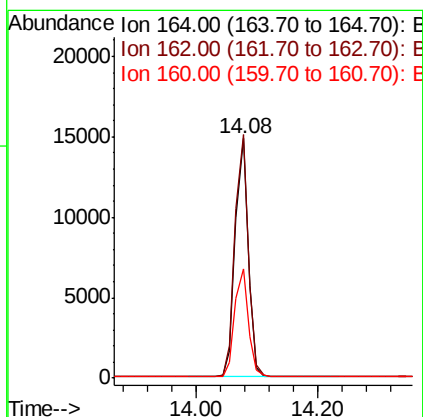







#13
 2,4,6-Tribromophenol
 Concen: 0.197 ng
 RT: 15.57 min Scan# 1444
 Delta R.T. -0.00 min
 Lab File: BN007143.D
 Acq: 13 Aug 2019 21:55

Instrument :
 BNA_N
 ClientSampleId :

Tot Ion:330 Resp: 2340
 Ion Ratio Lower Upper
 330 100
 332 0.0 0.0 0.0
 141 40.8 33.6 50.4

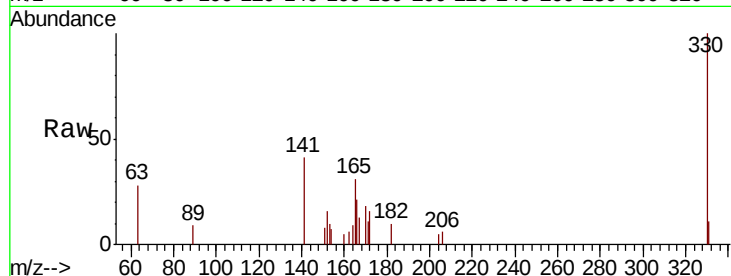


Abundance Ion 330.00 (329.70 to 330.70): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E


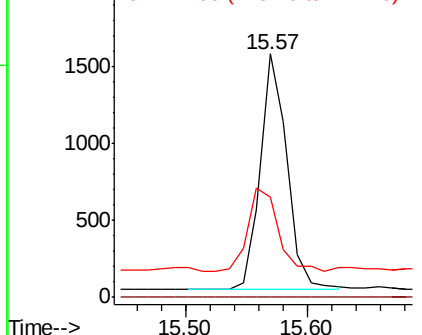



#14
 2-Fluorobiphenyl
 Concen: 0.176 ng
 RT: 12.71 min Scan# 1187
 Delta R.T. -0.00 min
 Lab File: BN007143.D
 Acq: 13 Aug 2019 21:55

Tgt Ion:172 Resp: 5624
 Ion Ratio Lower Upper
 172 100
 171 32.5 26.3 39.5
 170 20.0 17.0 25.4



Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

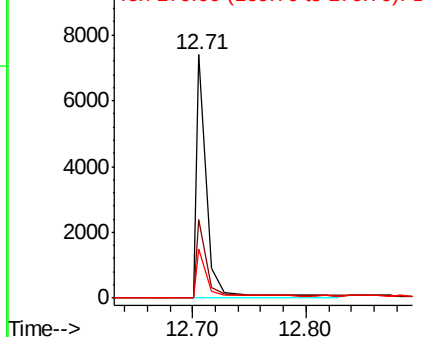

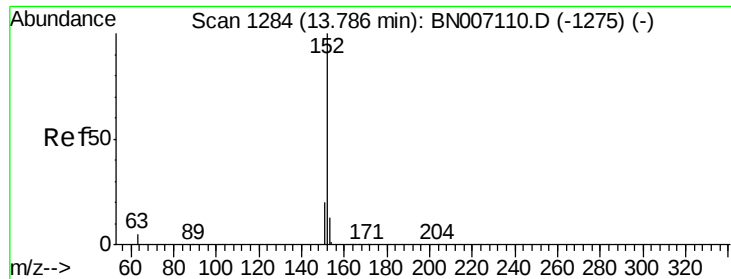

#15

Acenaphthylene

Concen: 0.109 ng

RT: 13.79 min Scan# 1284

Delta R.T. -0.00 min

Lab File: BN007143.D

Acq: 13 Aug 2019 21:55

Instrument :

BNA_N

ClientSampleId :


Tot Ion:152 Resp: 12546

Ion Ratio Lower Upper




152 100

151 20.8 15.8 23.6

153 12.6 10.4 15.6

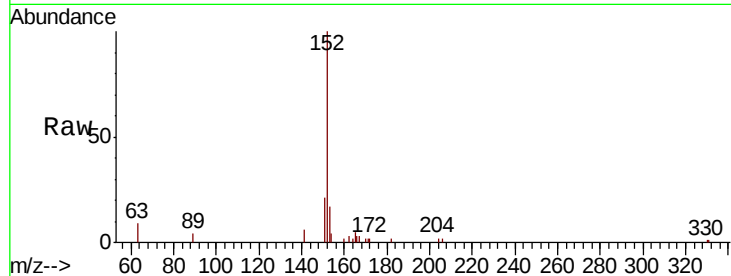

Abundance Ion 152.00 (151.70 to 152.70): E
Ion 151.00 (150.70 to 151.70): E
Ion 153.00 (152.70 to 153.70): E

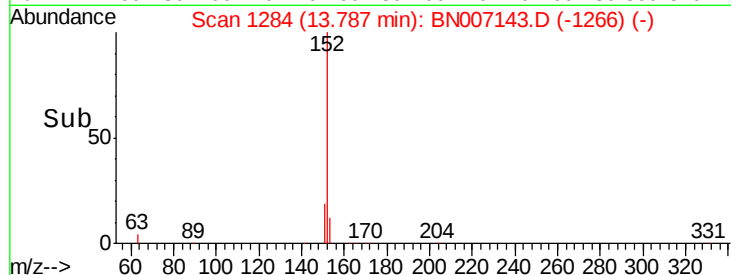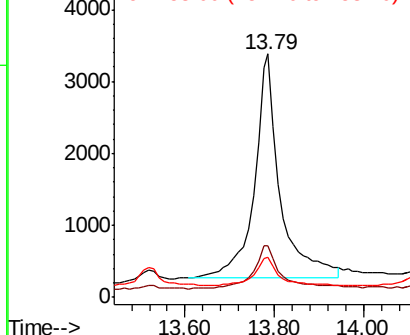

#17

Fluorene

Concen: 0.020 ng

RT: 15.14 min Scan# 1405

Delta R.T. -0.00 min

Lab File: BN007143.D

Acq: 13 Aug 2019 21:55


Tgt Ion:166 Resp: 2229

Ion Ratio Lower Upper



166 100


165 0.0 77.9 116.9#

167 11.0 10.9 16.3



Abundance Ion 166.00 (165.70 to 166.70): E
Ion 165.00 (164.70 to 165.70): E
Ion 167.00 (166.70 to 167.70): E



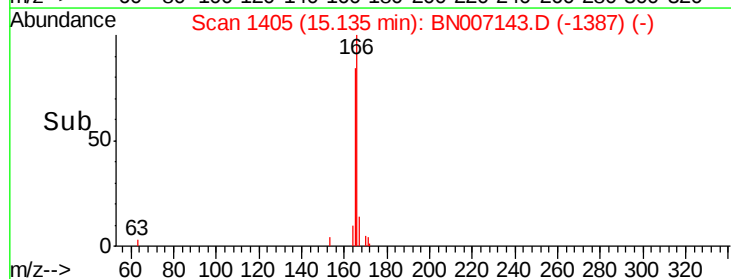
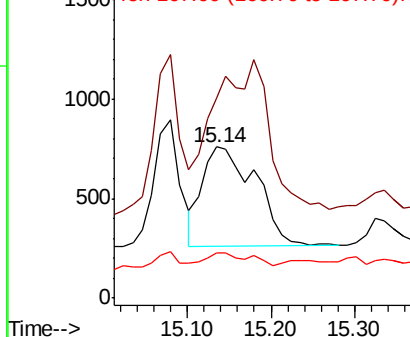




#18
Phenanthrene-d10
Concen: 0.400 ng
RT: 16.82 min Scan# 1560
Delta R.T. -0.00 min
Lab File: BN007143.D
Acq: 13 Aug 2019 21:55




Instrument :
BNA_N
ClientSampleId :


Tot Ion:188 Resp: 50034
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 8.3 7.8 11.6

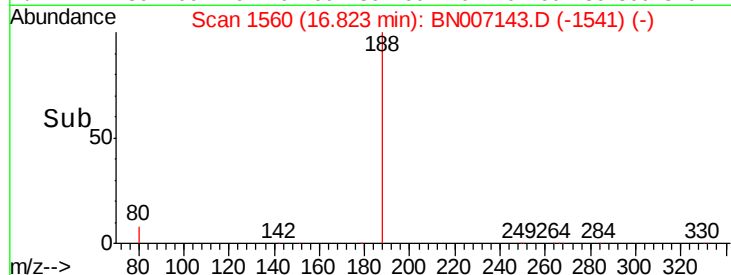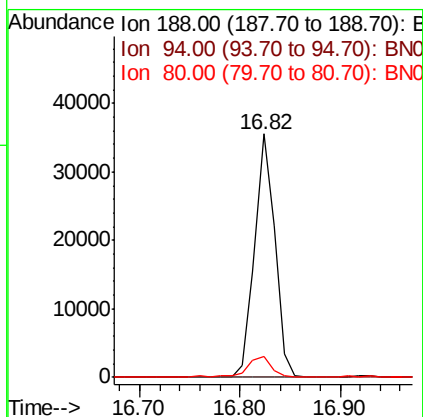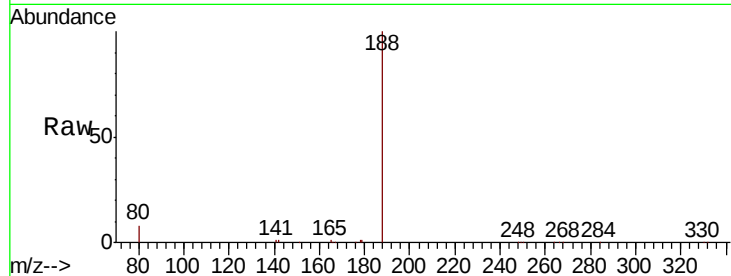

#24
Fluoranthene-d10
Concen: 0.288 ng
RT: 18.87 min Scan# 1844
Delta R.T. -0.01 min
Lab File: BN007143.D
Acq: 13 Aug 2019 21:55

Tgt Ion:212 Resp: 51174
Ion Ratio Lower Upper
212 100
106 10.4 8.2 12.2
104 5.8 4.5 6.7



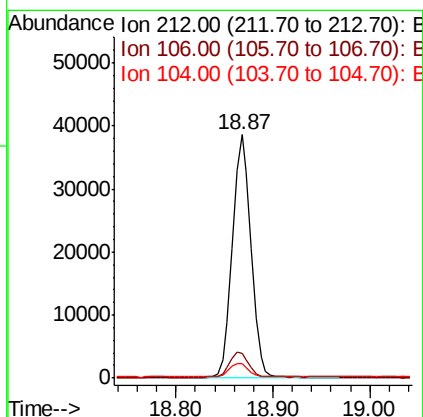





#26
 Chrysene-d12
 Concen: 0.400 ng
 RT: 21.05 min Scan# 2171
 Delta R.T. -0.01 min
 Lab File: BN007143.D
 Acq: 13 Aug 2019 21:55




Instrument :
 BNA_N
 ClientSampleId :




Tot Ion:240 Resp: 48198
 Ion Ratio Lower Upper
 240 100
 120 5.4 4.0 6.0
 236 26.5 21.3 31.9

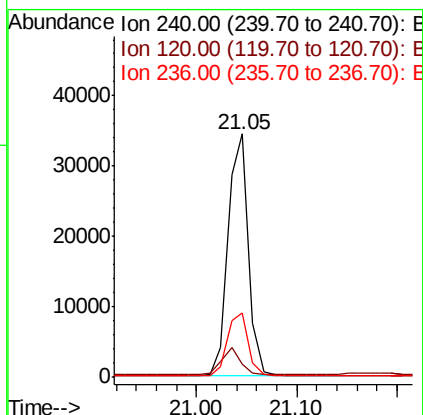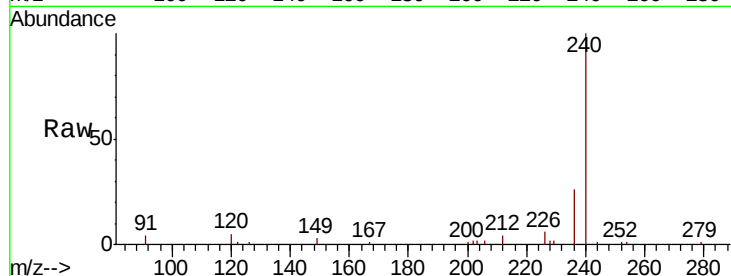

#28
 Terphenyl-d14
 Concen: 0.305 ng
 RT: 19.49 min Scan# 1969
 Delta R.T. -0.01 min
 Lab File: BN007143.D
 Acq: 13 Aug 2019 21:55

Tgt Ion:244 Resp: 40034
 Ion Ratio Lower Upper
 244 100
 212 7.9 6.2 9.2
 122 9.8 7.4 11.2

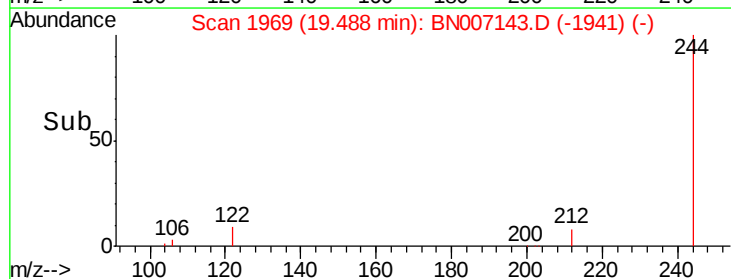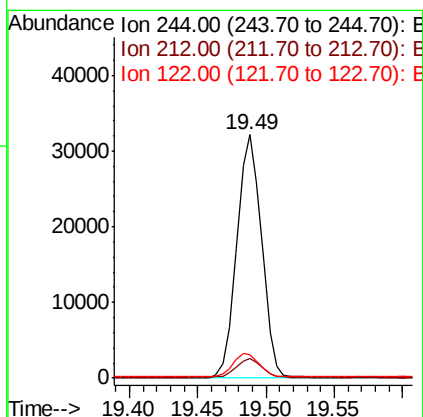

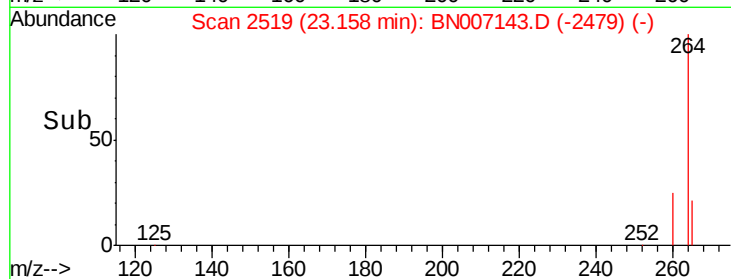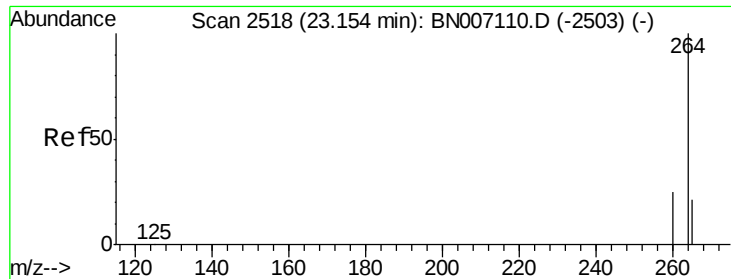

#32

Pervlene-d12

Concen: 0.400 ng

RT: 23.16 min Scan# 2519

Delta R.T. -0.01 min

Lab File: BN007143.D

Acq: 13 Aug 2019 21:55

Instrument :

BNA_N

ClientSampleId :

Tot Ion:264 Resp: 53495

Ion Ratio Lower Upper

264 100

260 25.2 19.8 29.8

265 32.4 26.2 39.4

