


#1




1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 7.43 min Scan# 547
Delta R.T. -0.00 min
Lab File: BN007160.D
Acq: 14 Aug 2019 09:21

Instrument :
BNA_N
ClientSampleId :

Tgt Ion:152 Resp: 8887
Ion Ratio Lower Upper
152 100
150 151.3 121.7 182.5
115 57.9 46.2 69.4

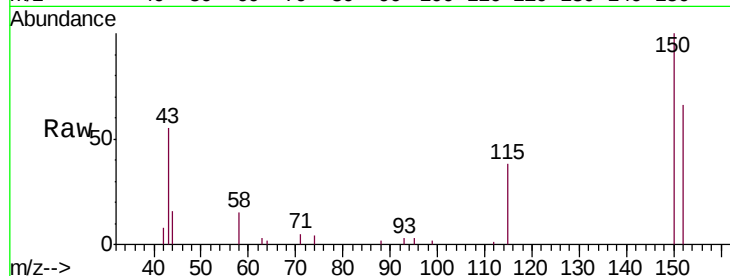


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

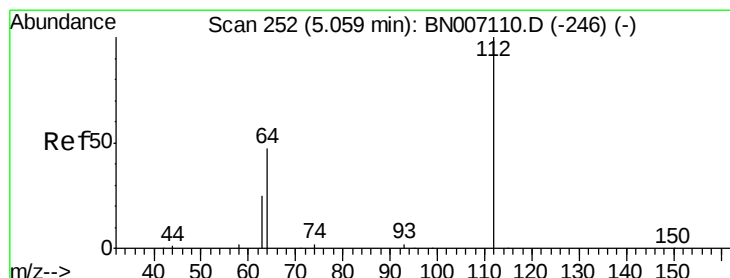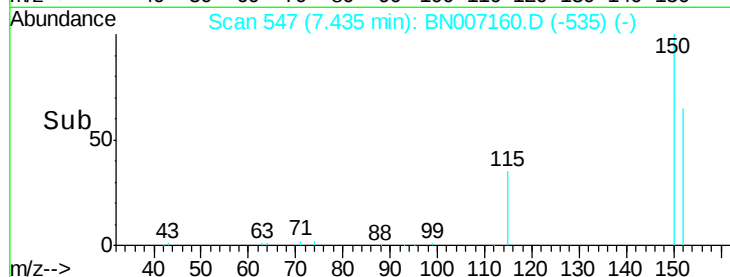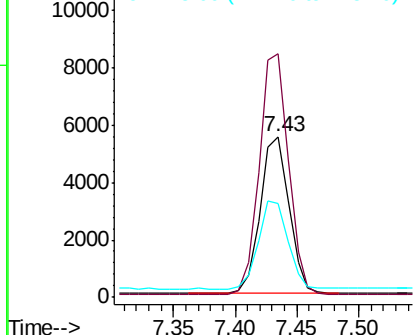

#3

2-Fluorophenol
Concen: 0.220 ng
RT: 5.06 min Scan# 252
Delta R.T. -0.00 min
Lab File: BN007160.D
Acq: 14 Aug 2019 09:21

Tgt Ion:112 Resp: 4705
Ion Ratio Lower Upper
112 100
64 52.3 42.6 63.8
63 27.7 22.2 33.2

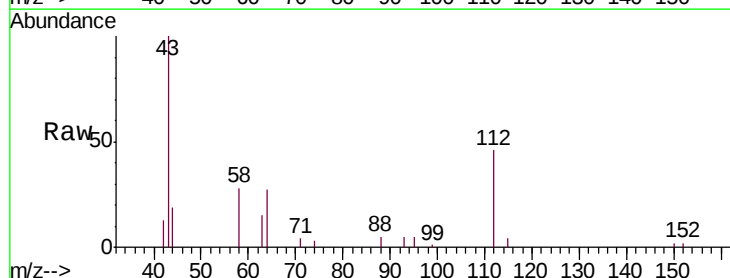

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BNC
Ion 63.00 (62.70 to 63.70): BNC

