

#4

Phenol-d6

Concen: 0.242 ng

RT: 6.62 min Scan# 446

Delta R.T. 0.01 min

Lab File: BN007160.D

Acq: 14 Aug 2019 09:21

Instrument :

BNA_N

ClientSampled :


Tgt Ion: 99 Resp: 6407

Ion Ratio Lower Upper

99 100

42 0.0 15.8 23.6#




71 36.4 27.0 40.4

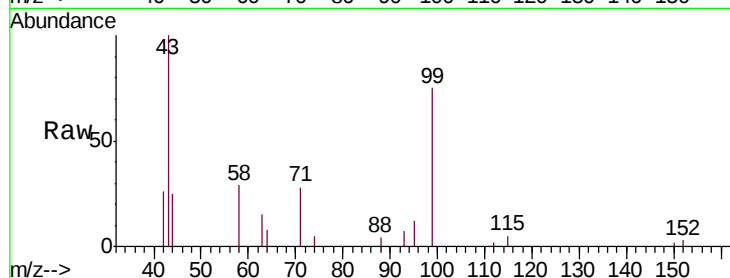

Abundance Ion 99.00 (98.70 to 99.70): BN007110.D (-439) (-)

Ion 42.00 (41.70 to 42.70): BN007110.D (-439) (-)

Ion 71.00 (70.70 to 71.70): BN007110.D (-439) (-)

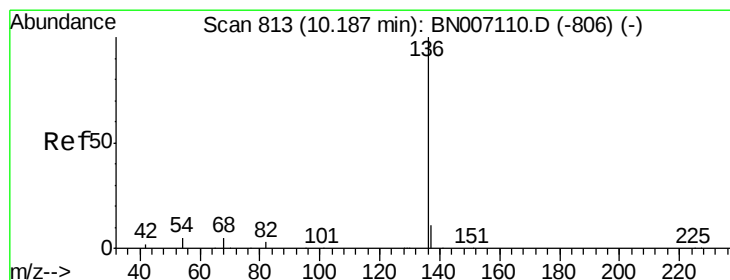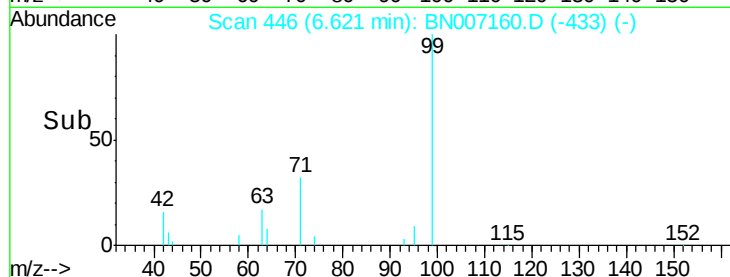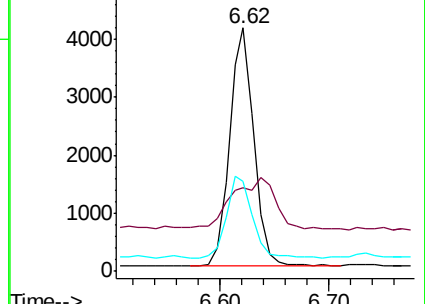

#6

Naphthalene-d8

Concen: 0.400 ng

RT: 10.19 min Scan# 813

Delta R.T. -0.00 min

Lab File: BN007160.D

Acq: 14 Aug 2019 09:21

Tgt Ion: 136 Resp: 35134


Ion Ratio Lower Upper

136 100

137 11.0 9.4 14.0

54 6.2 6.6 9.8#

68 5.9 6.0 9.0#

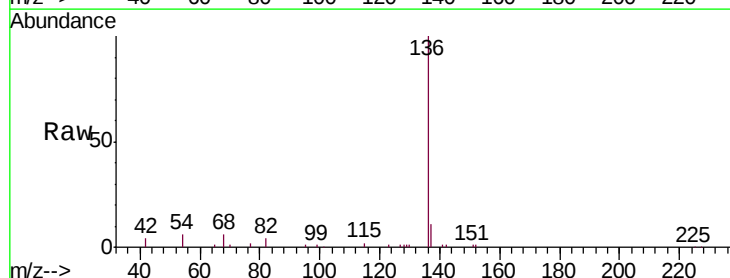

Abundance Ion 136.00 (135.70 to 136.70): BN007110.D (-806) (-)

Ion 137.00 (136.70 to 137.70): BN007110.D (-806) (-)

Ion 54.00 (53.70 to 54.70): BN007110.D (-806) (-)

Ion 68.00 (67.70 to 68.70): BN007110.D (-806) (-)

