
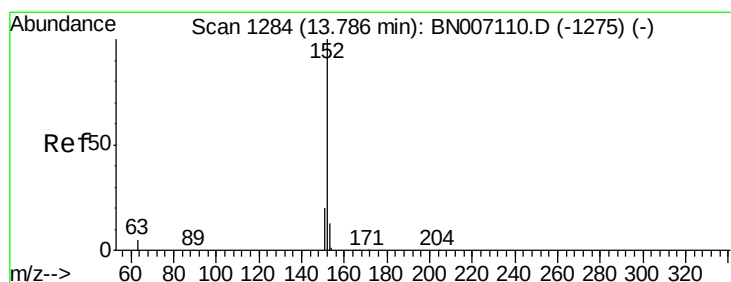
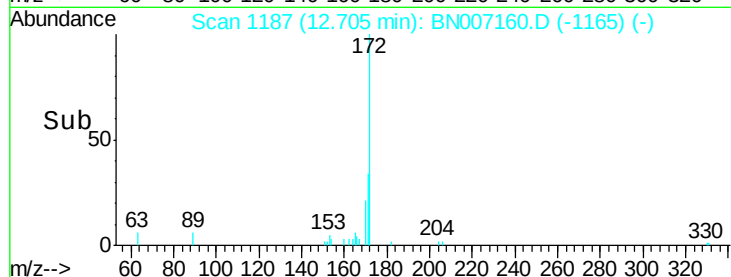
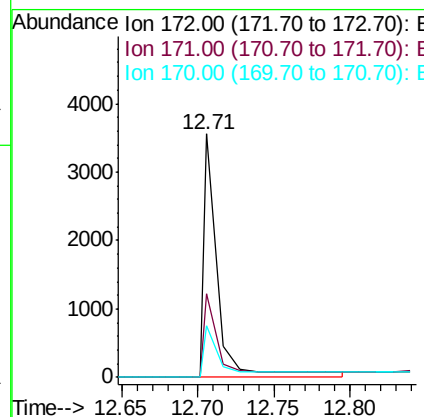


#14
2-Fluorobiphenyl
Concen: 0.093 ng
RT: 12.71 min Scan# 1187
Delta R.T. -0.00 min
Lab File: BN007160.D
Acq: 14 Aug 2019 09:21

Instrument :
BNA_N
ClientSampleId :

Tgt Ion:172 Resp: 2722
Ion Ratio Lower Upper
172 100
171 34.4 26.3 39.5
170 21.3 17.0 25.4

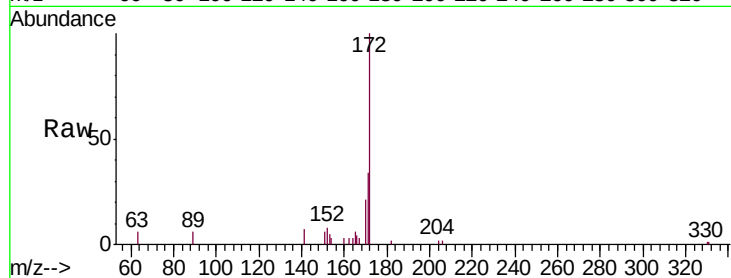

#15
Acenaphthylene
Concen: 0.852 ng
RT: 13.79 min Scan# 1284
Delta R.T. -0.00 min
Lab File: BN007160.D
Acq: 14 Aug 2019 09:21

Tgt Ion:152 Resp: 89522
Ion Ratio Lower Upper
152 100
151 19.1 15.8 23.6
153 13.8 10.4 15.6

