

#16

Acenaphthene

Concen: 0.295 ng

RT: 14.13 min Scan# 1315

Delta R.T. -0.01 min

Lab File: BN007160.D

Acq: 14 Aug 2019 09:21

Instrument :

BNA_N

ClientSampleId :





Tgt Ion:154 Resp: 19856

Ion Ratio Lower Upper

154 100

153 119.9 89.5 134.3

152 54.6 44.8 67.2

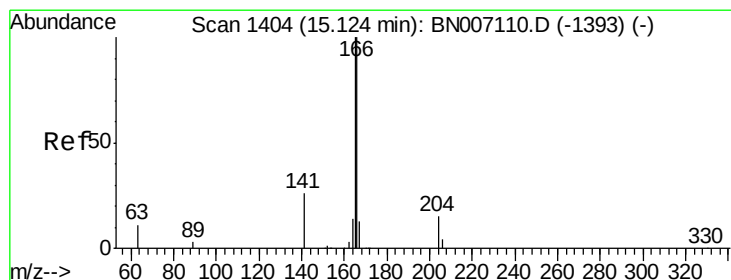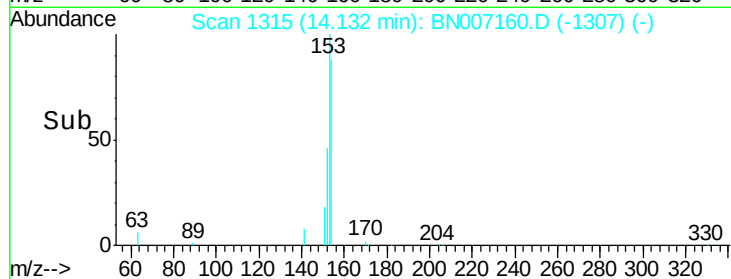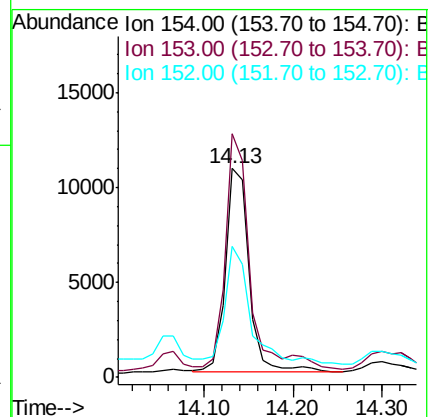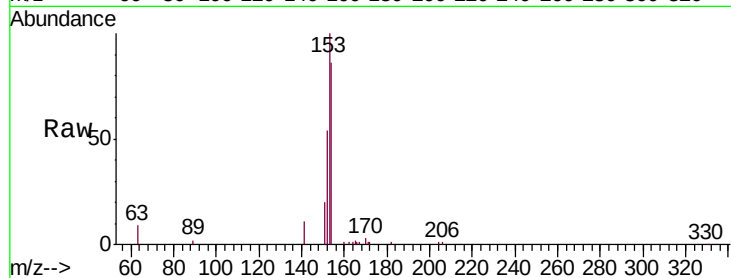

#17

Fluorene

Concen: 0.404 ng

RT: 15.14 min Scan# 1405

Delta R.T. -0.00 min

Lab File: BN007160.D

Acq: 14 Aug 2019 09:21

Tgt Ion:166 Resp: 40656

Ion Ratio Lower Upper

166 100

165 112.3 77.9 116.9

167 14.8 10.9 16.3

