

#18

Phenanthrene-d10

Concen: 0.400 ng

RT: 16.82 min Scan# 1560

Delta R.T. -0.00 min

Lab File: BN007160.D

Acq: 14 Aug 2019 09:21

Instrument :

BNA_N

ClientSampleId :





Tgt Ion:188 Resp: 44907

Ion Ratio Lower Upper

188 100

94 0.0 0.0 0.0

80 8.6 7.8 11.6

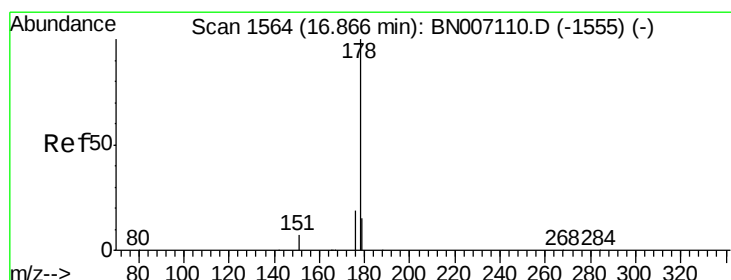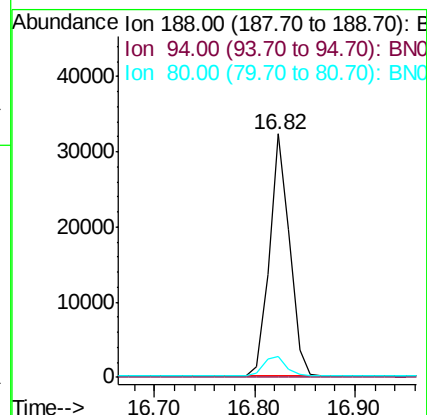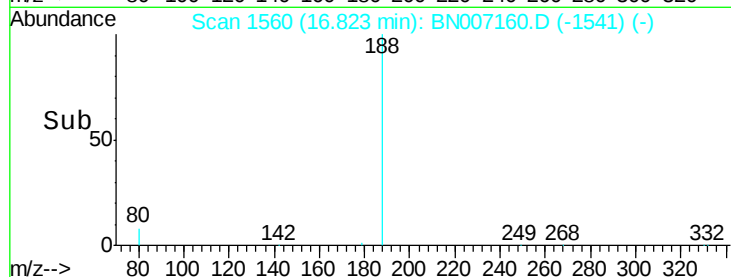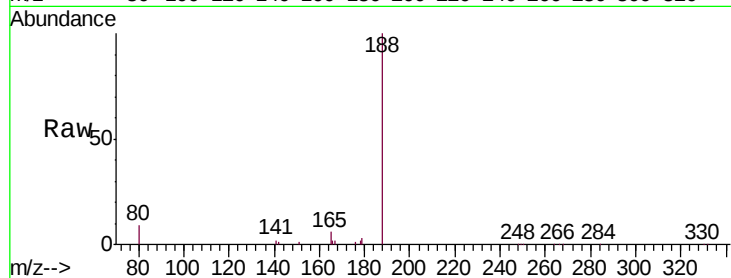

#22

Phenanthrene

Concen: 5.812 ng

RT: 16.87 min Scan# 1564

Delta R.T. -0.00 min

Lab File: BN007160.D

Acq: 14 Aug 2019 09:21

Tgt Ion:178 Resp: 782227

Ion Ratio Lower Upper

178 100

176 19.0 15.2 22.8

179 15.8 12.3 18.5

