

#23

Anthracene

Concen: 0.811 ng

RT: 16.96 min Scan# 1573

Delta R.T. -0.00 min

Lab File: BN007160.D

Acq: 14 Aug 2019 09:21

Instrument :

BNA_N

ClientSampleId :





Tgt Ion:178 Resp: 99696

Ion Ratio Lower Upper

178 100

176 18.3 14.6 21.8

179 18.4 12.5 18.7

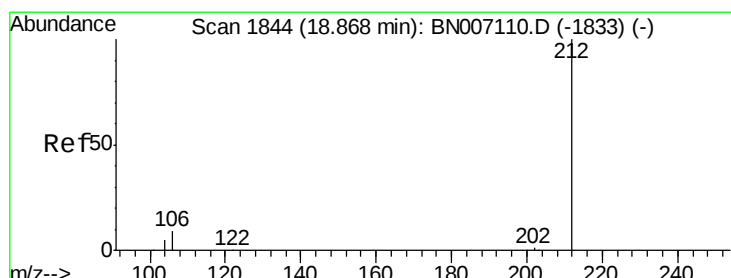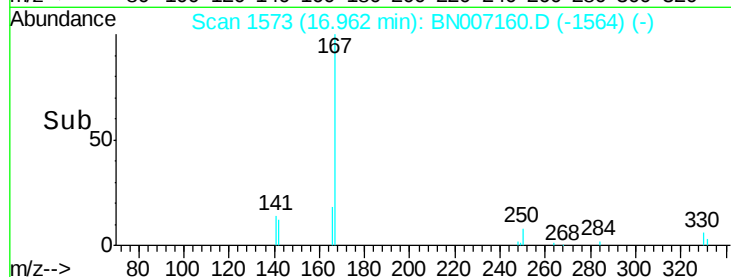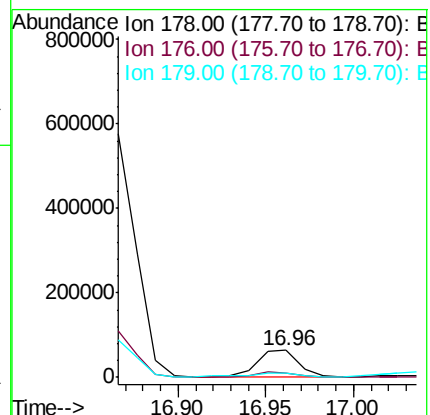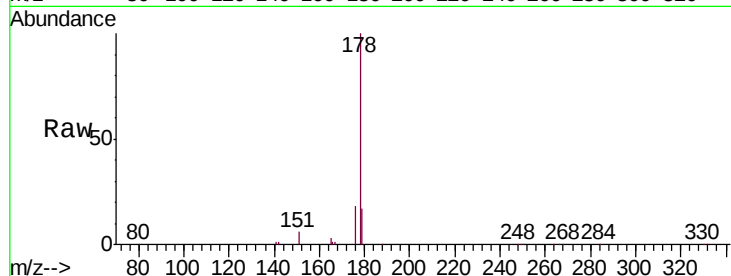

#24

Fluoranthene-d10

Concen: 0.137 ng

RT: 18.87 min Scan# 1845

Delta R.T. -0.00 min

Lab File: BN007160.D

Acq: 14 Aug 2019 09:21

Tgt Ion:212 Resp: 21862

Ion Ratio Lower Upper

212 100

106 9.6 8.2 12.2

104 8.8 4.5 6.7#

