

#29

Benzo(a)anthracene

Concen: 3.814 ng

RT: 21.08 min Scan# 2174

Delta R.T. 0.04 min

Lab File: BN007160.D

Acq: 14 Aug 2019 09:21

Instrument :

BNA_N

ClientSampleId :





Tgt Ion:228 Resp: 590576

Ion Ratio Lower Upper

228 100

226 31.6 21.8 32.6

229 22.3 15.6 23.4

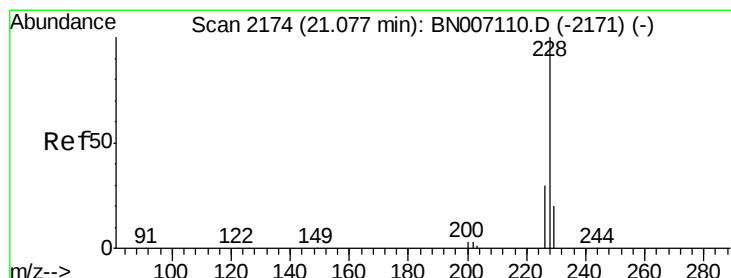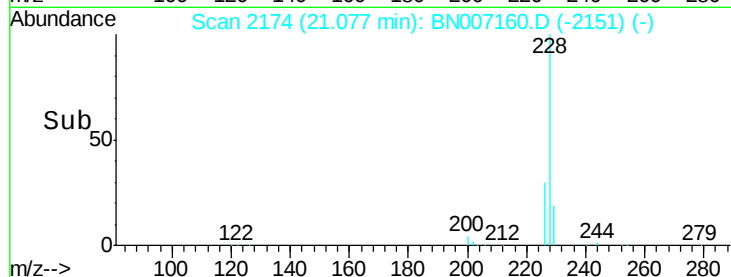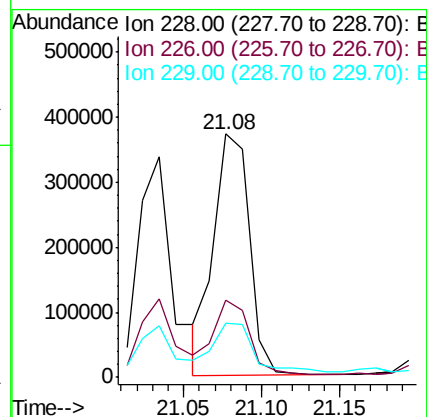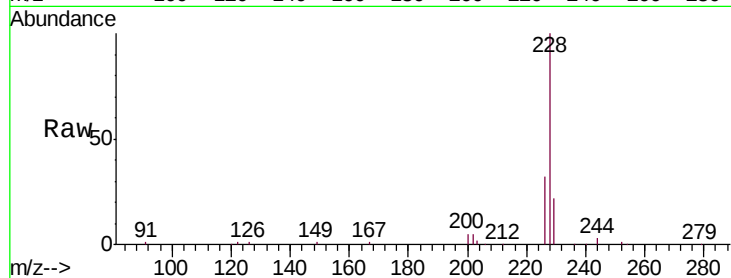

#30

Chrysene

Concen: 3.916 ng

RT: 21.08 min Scan# 2174

Delta R.T. -0.01 min

Lab File: BN007160.D

Acq: 14 Aug 2019 09:21

Tgt Ion:228 Resp: 589099

Ion Ratio Lower Upper

228 100

226 31.6 23.8 35.6

229 22.3 15.7 23.5

