

#33

Benzo(b)fluoranthene

Concen: 3.052 ng

RT: 22.54 min Scan# 2340

Delta R.T. -0.00 min

Lab File: BN007160.D

Acq: 14 Aug 2019 09:21

Instrument :

BNA_N

ClientSampleId :


Tgt Ion:252 Resp: 514043

Ion Ratio Lower Upper

252 100

253 23.4 18.2 27.2




125 9.8 7.4 11.0

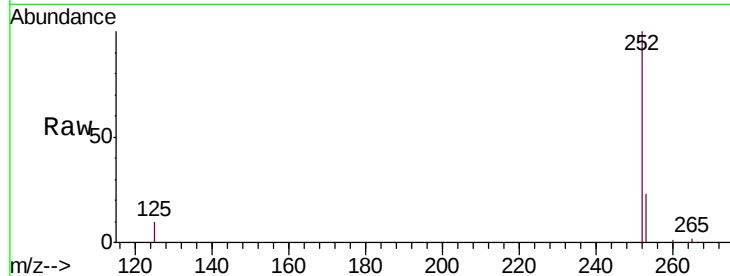

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

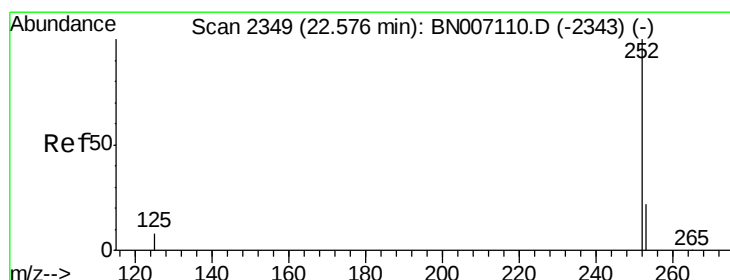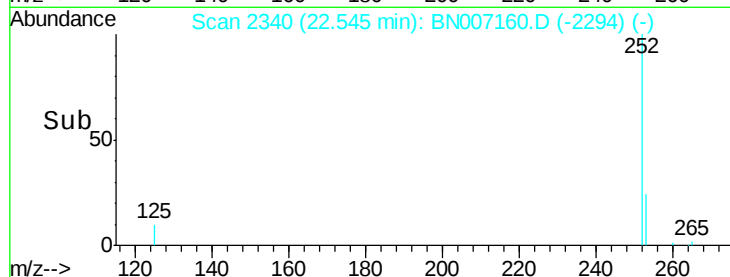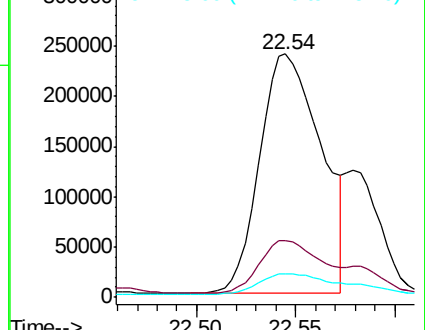

#34

Benzo(k)fluoranthene

Concen: 3.091 ng

RT: 22.54 min Scan# 2340

Delta R.T. -0.04 min

Lab File: BN007160.D

Acq: 14 Aug 2019 09:21


Tgt Ion:252 Resp: 514043

Ion Ratio Lower Upper

252 100

253 23.4 18.1 27.1

125 9.8 7.4 11.0

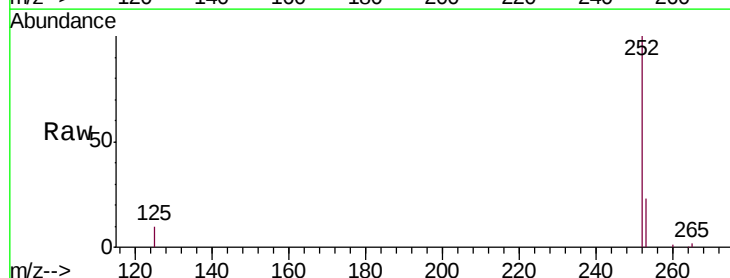

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

