

#35

Benzo(a)pyrene

Concen: 2.798 ng

RT: 23.08 min Scan# 2495

Delta R.T. -0.01 min

Lab File: BN007160.D

Acq: 14 Aug 2019 09:21

Instrument :

BNA_N

ClientSampleId :





Tgt Ion:252 Resp: 427164

Ion Ratio Lower Upper

252 100

253 23.2 18.5 27.7

125 9.9 8.2 12.4

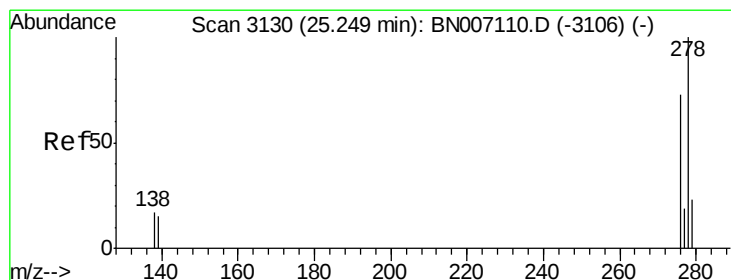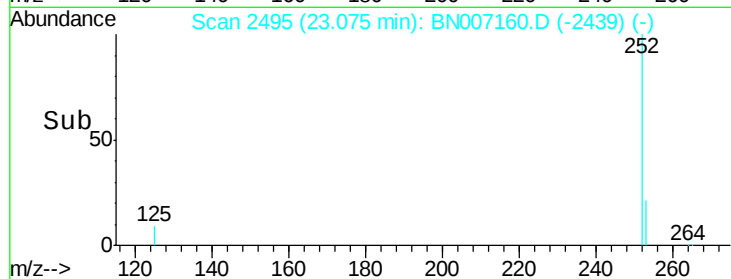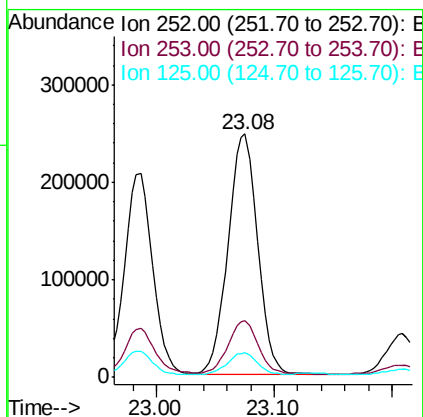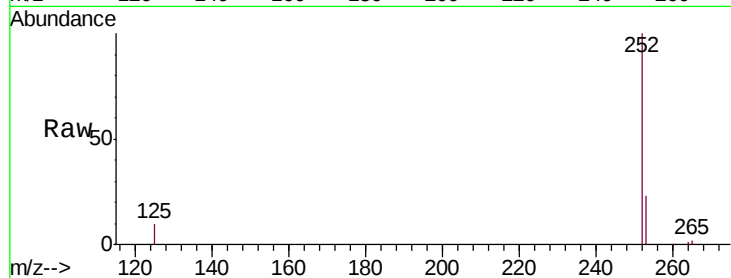

#36

Dibenzo(a,h)anthracene

Concen: 0.516 ng

RT: 25.25 min Scan# 3131

Delta R.T. -0.02 min

Lab File: BN007160.D

Acq: 14 Aug 2019 09:21

Tgt Ion:278 Resp: 78663

Ion Ratio Lower Upper

278 100

139 20.3 11.3 16.9#

279 33.5 19.3 28.9#

