


#1




1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 7.43 min Scan# 547
Delta R.T. -0.00 min
Lab File: BN007161.D
Acq: 14 Aug 2019 09:57

Instrument :
BNA_N
ClientSampleId :

Tgt Ion:152 Resp: 8767
Ion Ratio Lower Upper
152 100
150 149.8 121.7 182.5
115 59.3 46.2 69.4

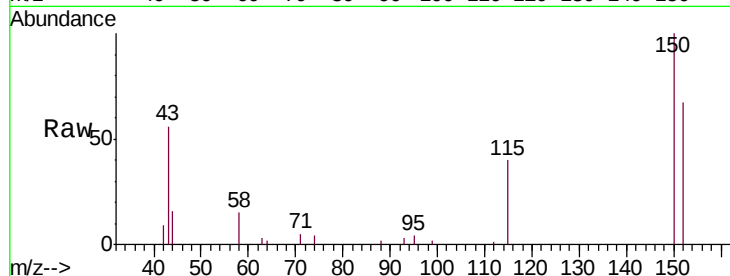


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

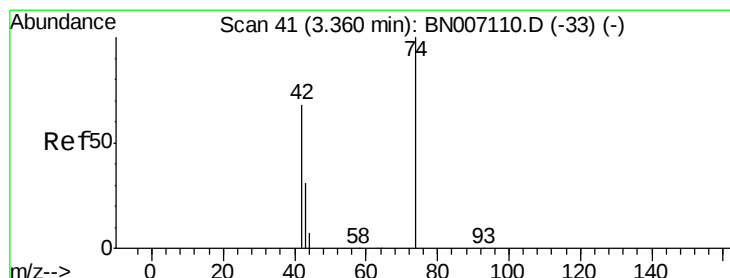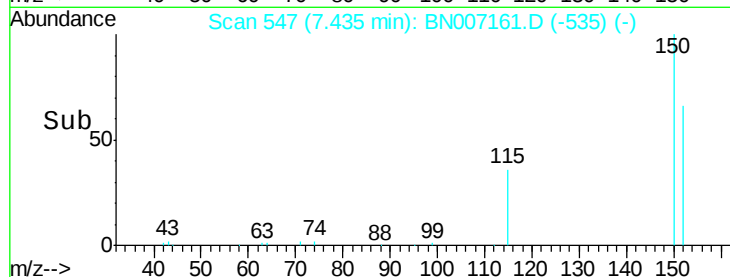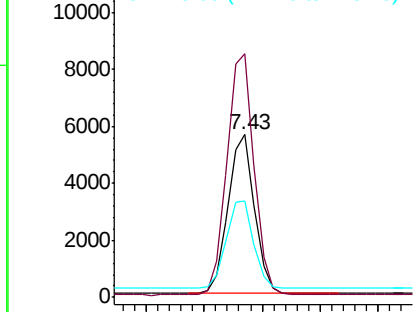

#2

n-Nitrosodimethylamine
Concen: 0.028 ng
RT: 3.39 min Scan# 45
Delta R.T. 0.03 min
Lab File: BN007161.D
Acq: 14 Aug 2019 09:57

Tgt Ion: 42 Resp: 164
Ion Ratio Lower Upper
42 100
74 4.9 110.6 166.0#
44 0.0 0.0 0.0

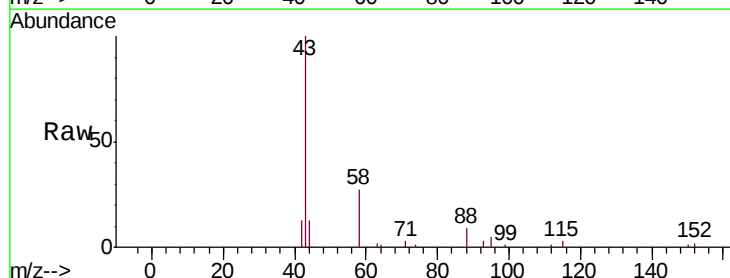

Abundance Ion 42.00 (41.70 to 42.70): BNC
Ion 74.00 (73.70 to 74.70): BNC
Ion 44.00 (43.70 to 44.70): BNC

