

#3

2-Fluorophenol

Concen: 0.226 ng

RT: 5.06 min Scan# 252

Delta R.T. -0.00 min

Lab File: BN007161.D

Acq: 14 Aug 2019 09:57

Instrument :

BNA_N

ClientSampleId :


Tgt Ion: 112 Resp: 4770

Ion Ratio Lower Upper

112 100

64 53.0 42.6 63.8




63 27.3 22.2 33.2

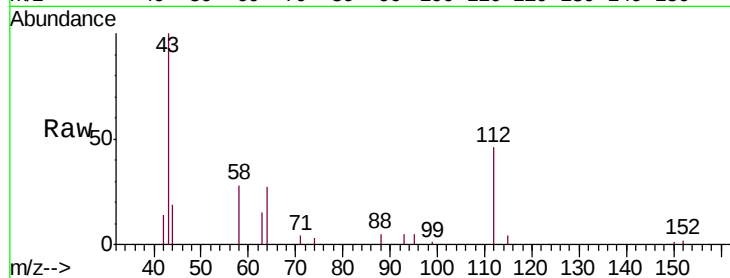

Abundance Ion 112.00 (111.70 to 112.70): BNC

Ion 64.00 (63.70 to 64.70): BNC

Ion 63.00 (62.70 to 63.70): BNC

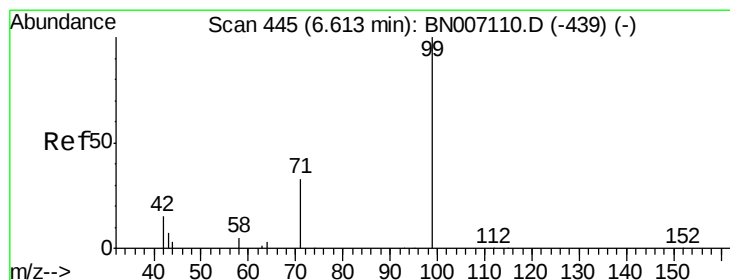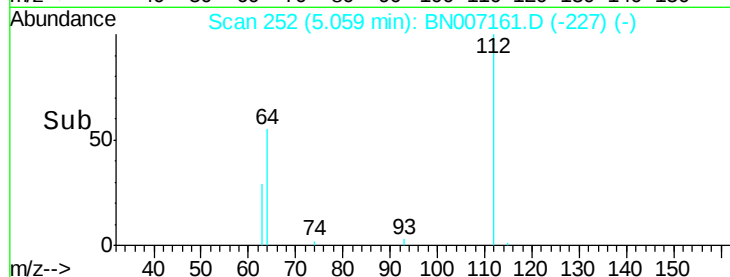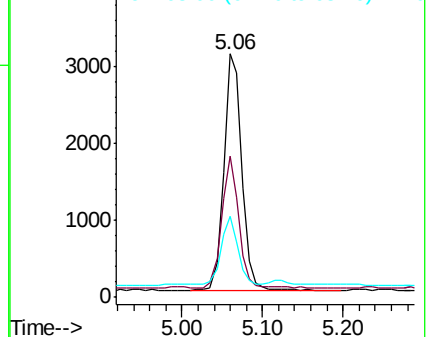

#4

Phenol-d6

Concen: 0.241 ng

RT: 6.62 min Scan# 446

Delta R.T. 0.01 min

Lab File: BN007161.D

Acq: 14 Aug 2019 09:57


Tgt Ion: 99 Resp: 6296

Ion Ratio Lower Upper

99 100

42 0.0 15.8 23.6#

71 35.8 27.0 40.4

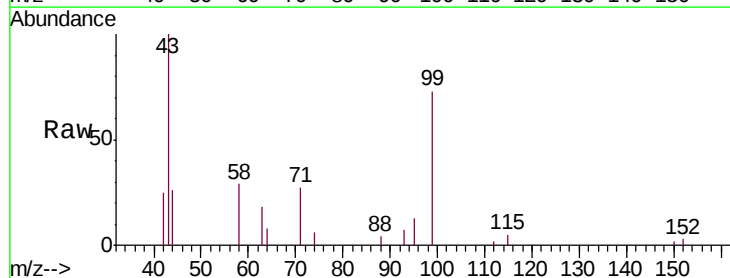

Abundance Ion 99.00 (98.70 to 99.70): BNC

Ion 42.00 (41.70 to 42.70): BNC

Ion 71.00 (70.70 to 71.70): BNC

