
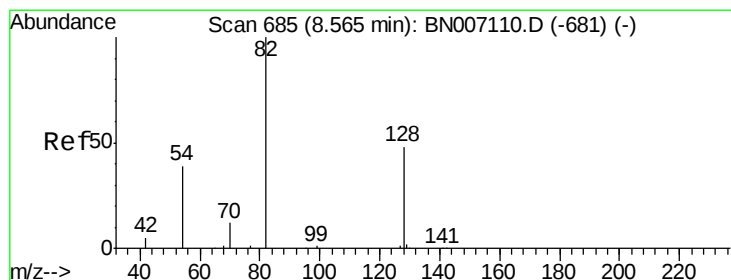
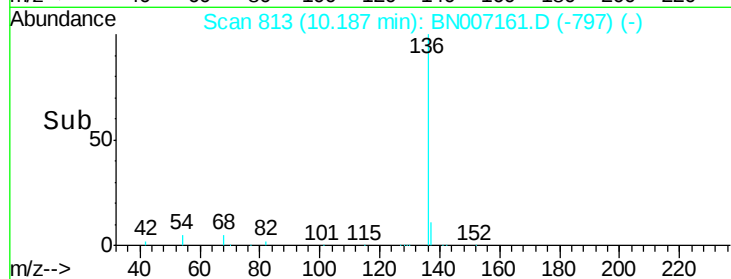
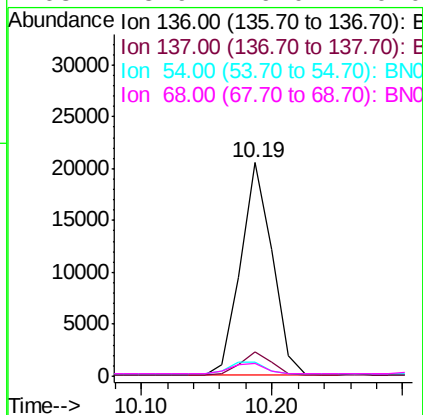


#6
Naphthalene-d8
Concen: 0.400 ng
RT: 10.19 min Scan# 813
Delta R.T. -0.00 min
Lab File: BN007161.D
Acq: 14 Aug 2019 09:57

Instrument :
BNA_N
ClientSampleId :

Tgt Ion:	136	Resp:	34359
Ion	Ratio	Lower	Upper
136	100		
137	11.2	9.4	14.0
54	6.4	6.6	9.8#
68	5.9	6.0	9.0#

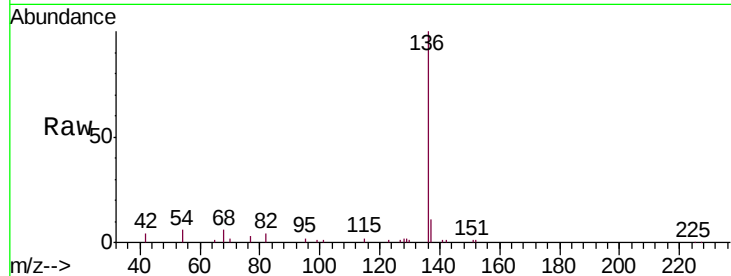

#7
Nitrobenzene-d5
Concen: 0.185 ng
RT: 8.56 min Scan# 685
Delta R.T. -0.00 min
Lab File: BN007161.D
Acq: 14 Aug 2019 09:57

Tgt Ion:	82	Resp:	5124
Ion	Ratio	Lower	Upper
82	100		
128	51.6	34.6	51.8
54	43.9	36.2	54.4

