
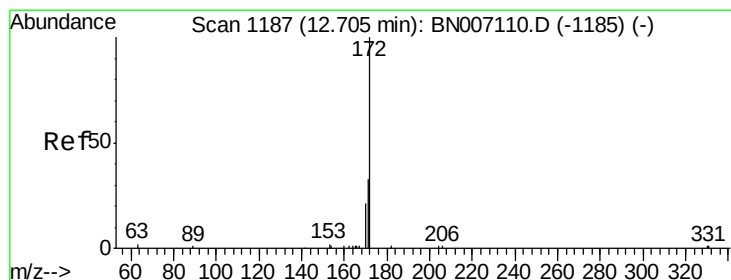
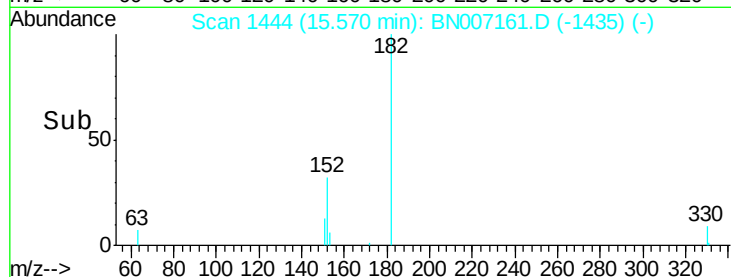
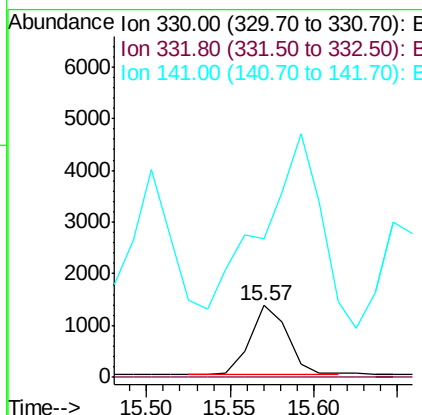


#13
 2,4,6-Tribromophenol
 Concen: 0.176 ng
 RT: 15.57 min Scan# 1444
 Delta R.T. -0.00 min
 Lab File: BN007161.D
 Acq: 14 Aug 2019 09:57

Instrument :
 BNA_N
 ClientSampleId :

Tgt Ion: 330 Resp: 2027
 Ion Ratio Lower Upper
 330 100
 332 0.0 0.0 0.0
 141 0.0 33.6 50.4#

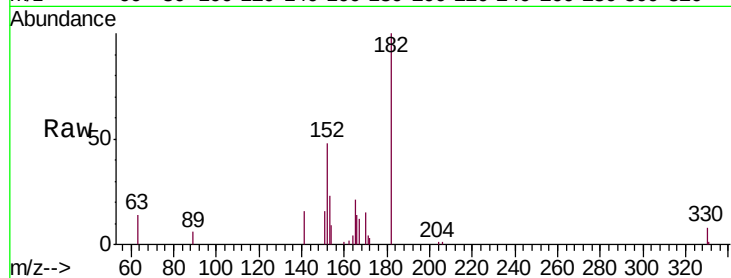

#14
 2-Fluorobiphenyl
 Concen: 0.086 ng
 RT: 12.71 min Scan# 1187
 Delta R.T. -0.00 min
 Lab File: BN007161.D
 Acq: 14 Aug 2019 09:57

Tgt Ion: 172 Resp: 2680
 Ion Ratio Lower Upper
 172 100
 171 33.9 26.3 39.5
 170 22.2 17.0 25.4

