

#17

Fluorene

Concen: 1.673 ng

RT: 15.14 min Scan# 1405

Delta R.T. -0.00 min

Lab File: BN007161.D

Acq: 14 Aug 2019 09:57

Instrument :

BNA\_N

ClientSampleId :


Tgt Ion:166 Resp: 179708

Ion Ratio Lower Upper

166 100

165 107.4 77.9 116.9




167 17.0 10.9 16.3#

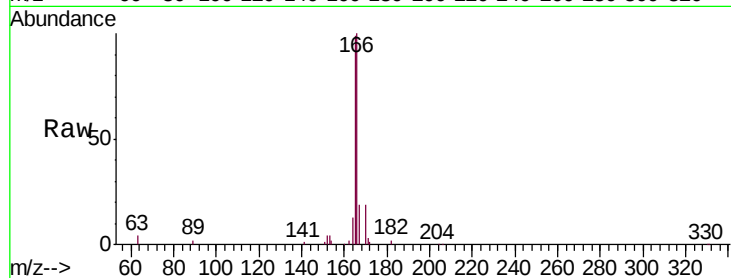

Abundance Ion 166.00 (165.70 to 166.70): E

Ion 165.00 (164.70 to 165.70): E

Ion 167.00 (166.70 to 167.70): E

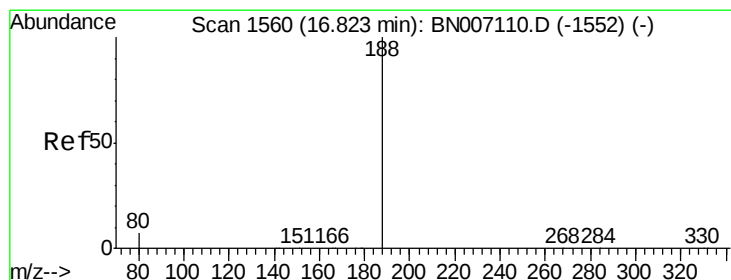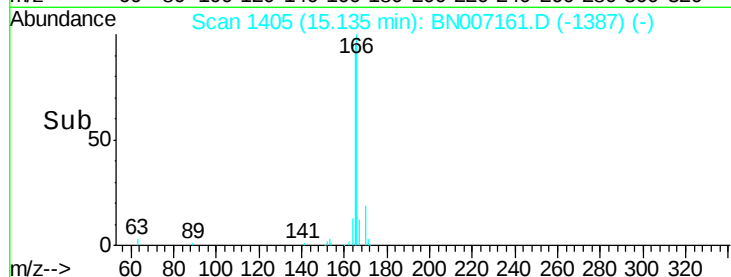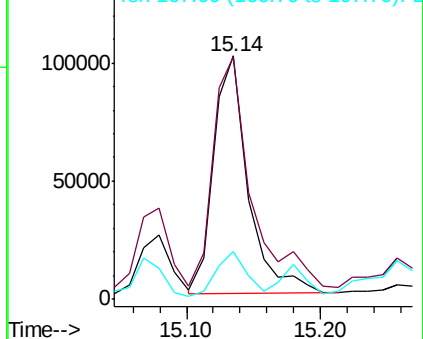

#18

Phenanthrene-d10

Concen: 0.400 ng

RT: 16.82 min Scan# 1560

Delta R.T. -0.00 min

Lab File: BN007161.D

Acq: 14 Aug 2019 09:57


Tgt Ion:188 Resp: 44070

Ion Ratio Lower Upper

188 100

94 0.0 0.0 0.0

80 9.4 7.8 11.6

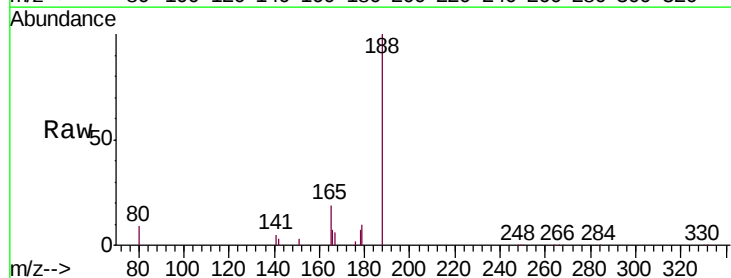

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BNC

Ion 80.00 (79.70 to 80.70): BNC

