

#24

Fluoranthene-d10

Concen: 0.144 ng

RT: 18.87 min Scan# 1845

Delta R.T. -0.00 min

Lab File: BN007161.D

Acq: 14 Aug 2019 09:57

Instrument :

BNA_N

ClientSampleId :


Tgt Ion:212 Resp: 22432

Ion Ratio Lower Upper

212 100

106 12.2 8.2 12.2




104 12.2 4.5 6.7#

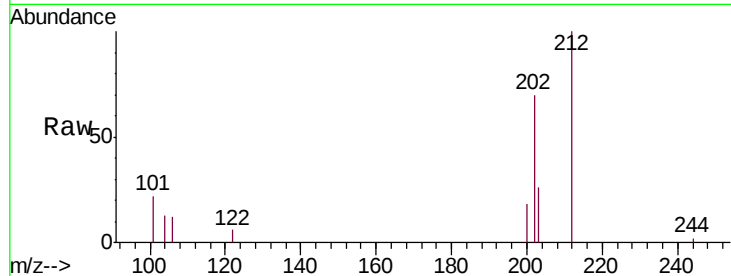

Abundance Ion 212.00 (211.70 to 212.70): E

Ion 106.00 (105.70 to 106.70): E

Ion 104.00 (103.70 to 104.70): E

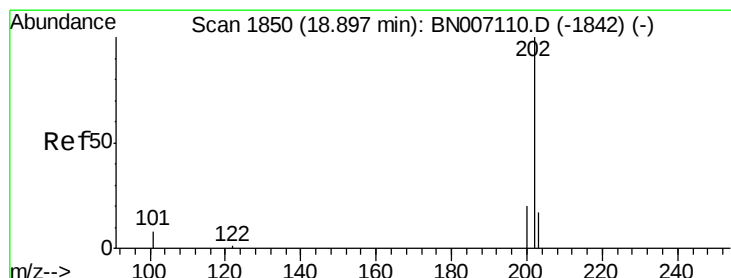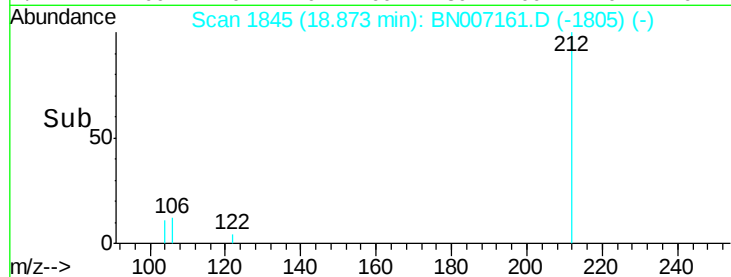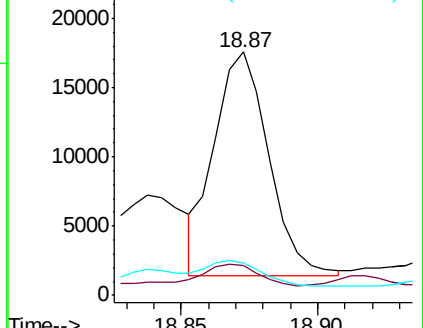

#25

Fluoranthene

Concen: 18.626 ng

RT: 18.90 min Scan# 1851

Delta R.T. -0.00 min

Lab File: BN007161.D

Acq: 14 Aug 2019 09:57


Tgt Ion:202 Resp: 3146853

Ion Ratio Lower Upper

202 100

101 9.2 7.0 10.4

203 18.4 13.8 20.8

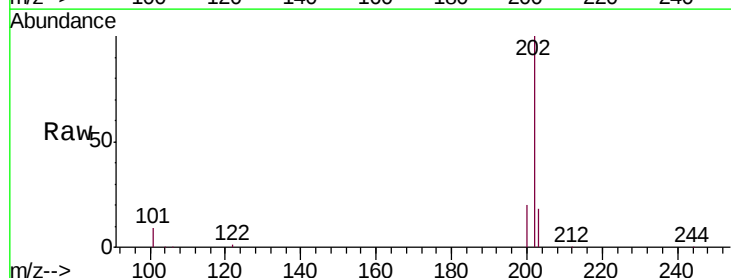

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 203.00 (202.70 to 203.70): E

