
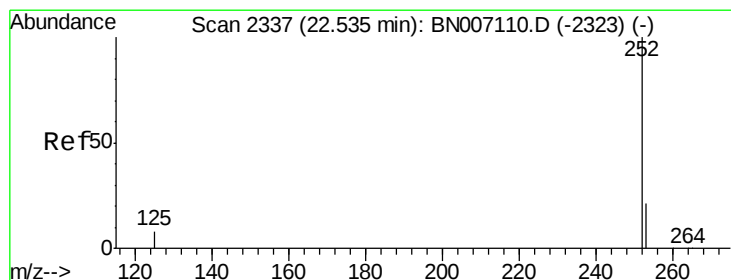
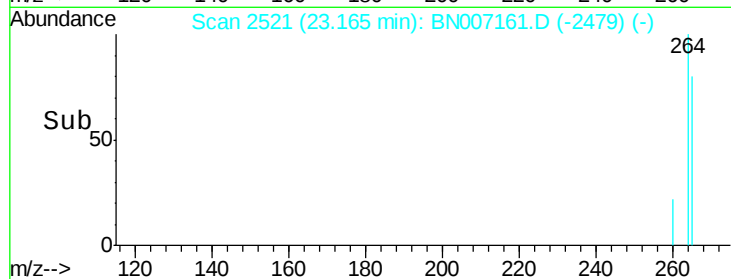
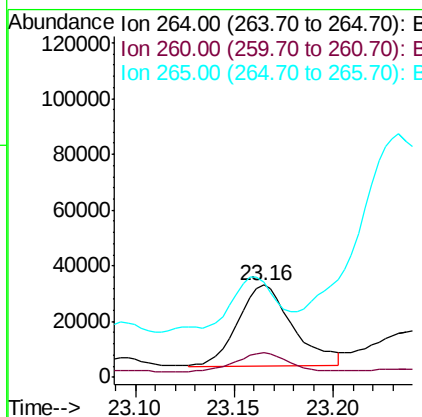


#32
 Perylene-d12
 Concen: 0.400 ng
 RT: 23.16 min Scan# 2521
 Delta R.T. -0.01 min
 Lab File: BN007161.D
 Acq: 14 Aug 2019 09:57

Instrument :
 BNA_N
 ClientSampleId :

Tgt Ion: 264 Resp: 55501
 Ion Ratio Lower Upper
 264 100
 260 26.9 19.8 29.8
 265 102.4 26.2 39.4#

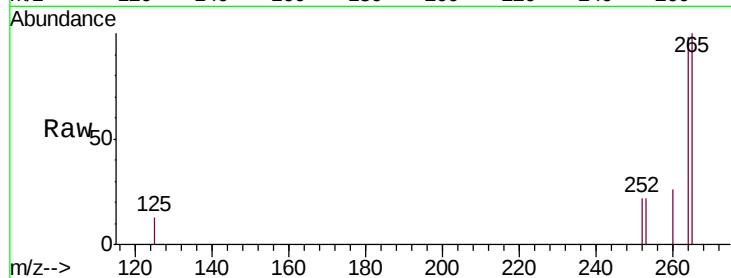

#33
 Benzo(b)fluoranthene
 Concen: 13.176 ng
 RT: 22.55 min Scan# 2341
 Delta R.T. -0.00 min
 Lab File: BN007161.D
 Acq: 14 Aug 2019 09:57

Tgt Ion: 252 Resp: 2507531
 Ion Ratio Lower Upper
 252 100
 253 23.2 18.2 27.2
 125 9.3 7.4 11.0

