
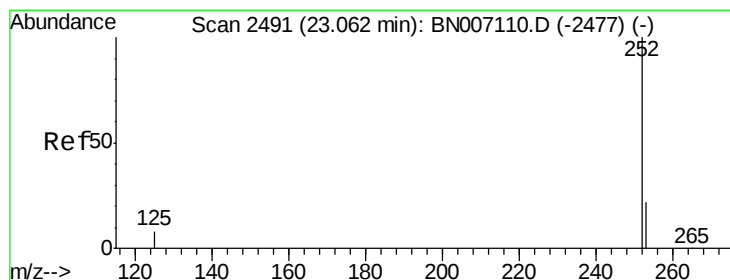
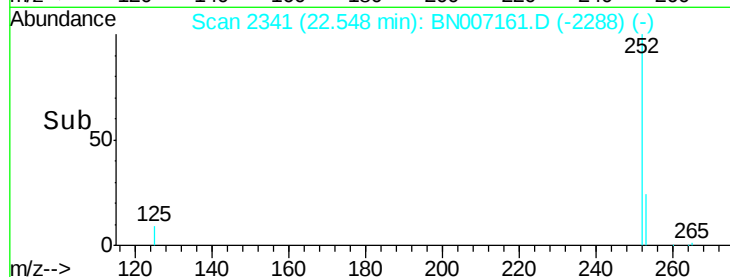
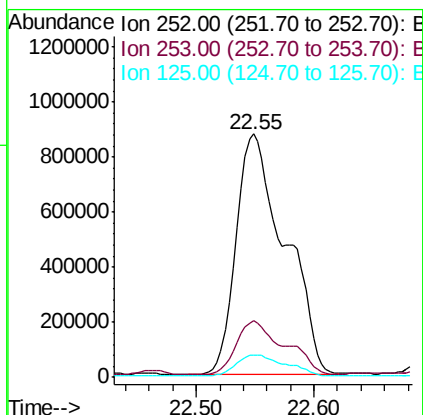


#34
Benzo(k)fluoranthene
Concen: 13.341 ng
RT: 22.55 min Scan# 2341
Delta R.T. -0.04 min
Lab File: BN007161.D
Acq: 14 Aug 2019 09:57

Instrument :
BNA_N
ClientSampleId :

Tgt Ion:252 Resp: 2507531
Ion Ratio Lower Upper
252 100
253 23.2 18.1 27.1
125 9.3 7.4 11.0

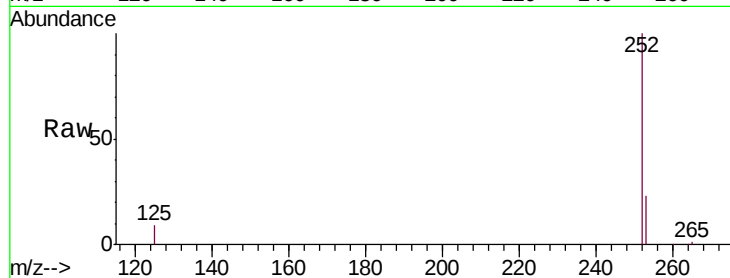

#35
Benzo(a)pyrene
Concen: 10.232 ng
RT: 23.08 min Scan# 2495
Delta R.T. -0.01 min
Lab File: BN007161.D
Acq: 14 Aug 2019 09:57

Tgt Ion:252 Resp: 1765431
Ion Ratio Lower Upper
252 100
253 22.7 18.5 27.7
125 9.3 8.2 12.4

