

#36

Dibenzo(a,h)anthracene

Concen: 1.851 ng

RT: 25.26 min Scan# 3132

Delta R.T. -0.02 min

Lab File: BN007161.D

Acq: 14 Aug 2019 09:57

Instrument :

BNA_N

ClientSampleId :


Tgt Ion:278 Resp: 318705

Ion Ratio Lower Upper

278 100

139 16.5 11.3 16.9




279 30.0 19.3 28.9#

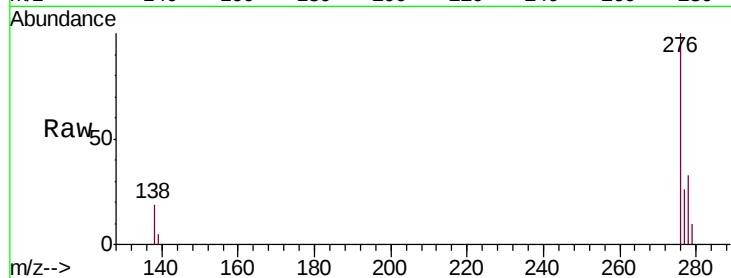

Abundance Ion 278.00 (277.70 to 278.70): E

Ion 139.00 (138.70 to 139.70): E

Ion 279.00 (278.70 to 279.70): E

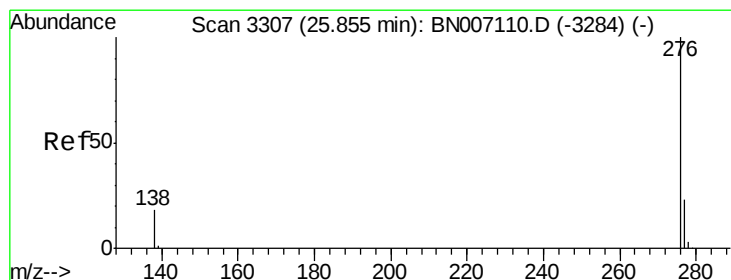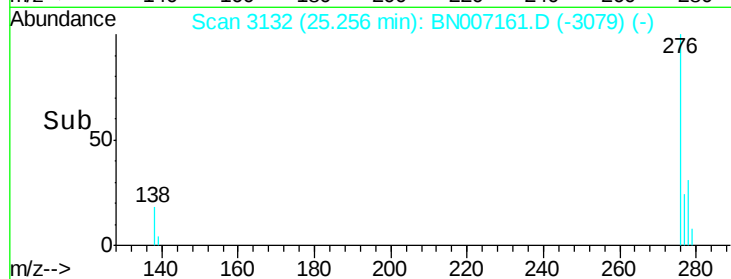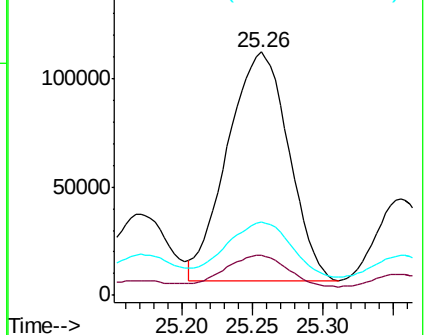

#37

Benzo(g,h,i)perylene

Concen: 6.940 ng

RT: 25.88 min Scan# 3314

Delta R.T. -0.00 min

Lab File: BN007161.D

Acq: 14 Aug 2019 09:57


Tgt Ion:276 Resp: 1229010

Ion Ratio Lower Upper

276 100

277 24.6 19.8 29.8

138 18.7 14.6 22.0

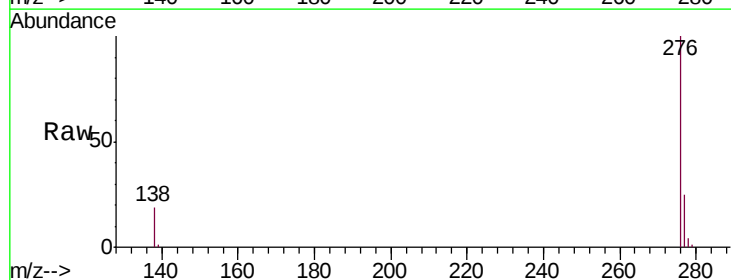

Abundance Ion 276.00 (275.70 to 276.70): E

Ion 277.00 (276.70 to 277.70): E

Ion 138.00 (137.70 to 138.70): E

