

#7

Nitrobenzene-d5

Concen: 0.218 ng

RT: 8.56 min Scan# 685

Delta R.T. -0.00 min

Lab File: BN007162.D

Acq: 14 Aug 2019 10:33

Instrument :

BNA_N

ClientSampled :


Tgt Ion: 82 Resp: 5736

Ion Ratio Lower Upper

82 100

128 50.9 34.6 51.8

54 42.4 36.2 54.4

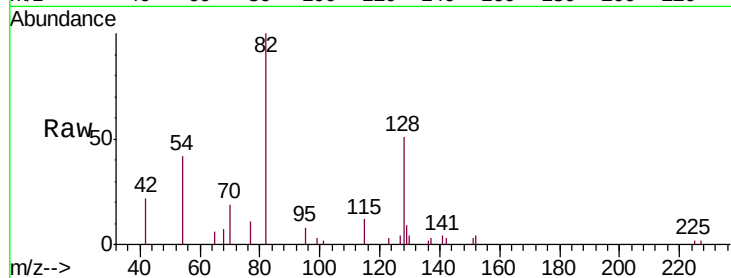


Abundance Ion 82.00 (81.70 to 82.70): BN007110.D (-681) (-)

Ion 128.00 (127.70 to 128.70): BN007110.D (-681) (-)

Ion 54.00 (53.70 to 54.70): BN007110.D (-681) (-)

Time-->

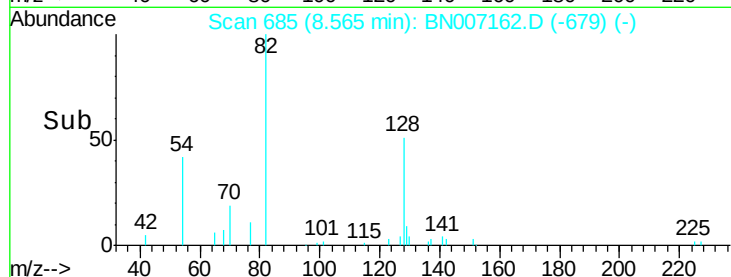


Abundance

Ion 82.00 (81.70 to 82.70): BN007162.D (-679) (-)

Ion 128.00 (127.70 to 128.70): BN007162.D (-679) (-)

Ion 54.00 (53.70 to 54.70): BN007162.D (-679) (-)

Time-->

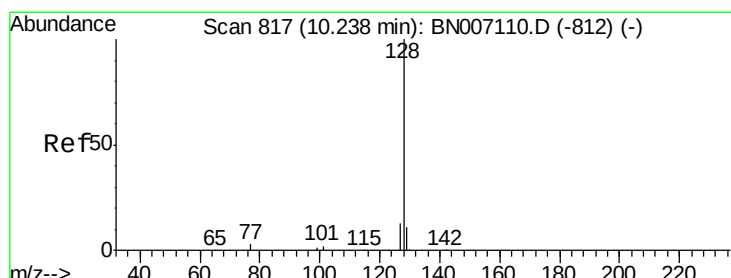

#8

Naphthalene

Concen: 0.254 ng

RT: 10.24 min Scan# 817

Delta R.T. -0.00 min

Lab File: BN007162.D

Acq: 14 Aug 2019 10:33


Tgt Ion: 128 Resp: 23315

Ion Ratio Lower Upper

128 100

129 12.2 9.4 14.2

127 13.8 11.0 16.6

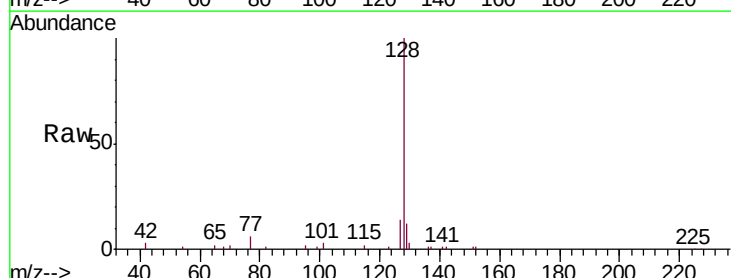


Abundance Ion 128.00 (127.70 to 128.70): BN007110.D (-812) (-)

Ion 129.00 (128.70 to 129.70): BN007110.D (-812) (-)

Ion 127.00 (126.70 to 127.70): BN007110.D (-812) (-)

Time-->

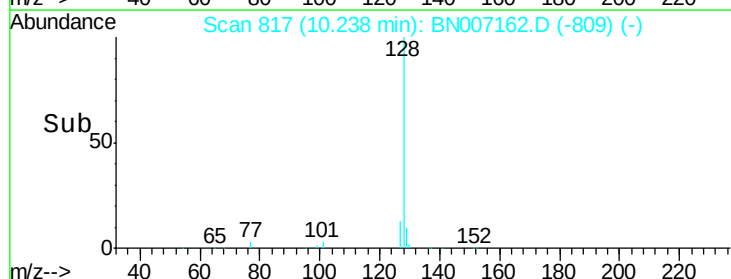

Abundance

Ion 128.00 (127.70 to 128.70): BN007162.D (-809) (-)

Ion 129.00 (128.70 to 129.70): BN007162.D (-809) (-)

Ion 127.00 (126.70 to 127.70): BN007162.D (-809) (-)

Time-->