
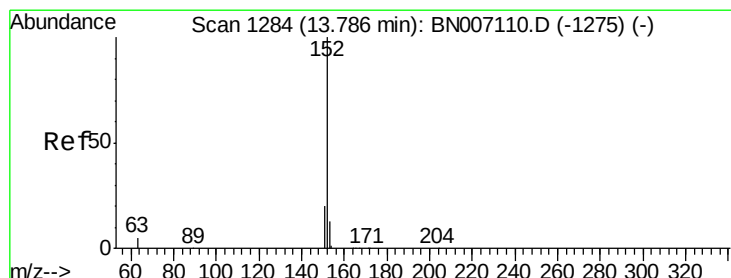
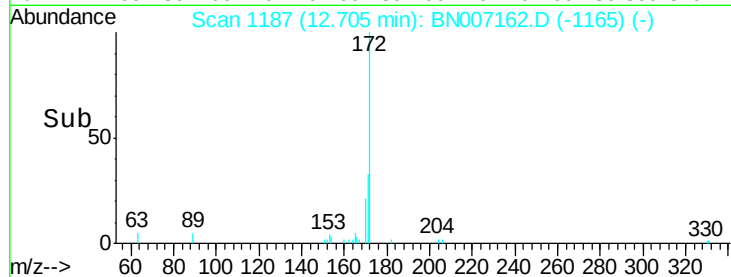
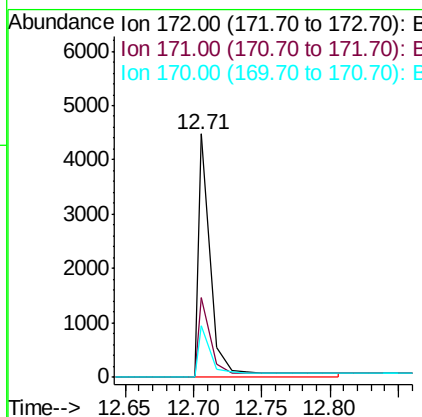


#14  
2-Fluorobiphenyl  
Concen: 0.123 ng  
RT: 12.71 min Scan# 1187  
Delta R.T. -0.00 min  
Lab File: BN007162.D  
Acq: 14 Aug 2019 10:33

Instrument :  
BNA\_N  
ClientSampleId :

Tgt Ion:172 Resp: 3418  
Ion Ratio Lower Upper  
172 100  
171 33.0 26.3 39.5  
170 21.3 17.0 25.4

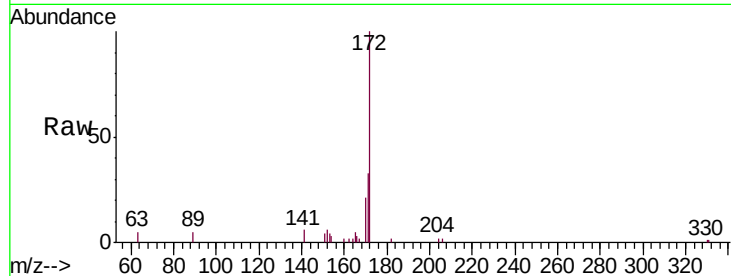

#15  
Acenaphthylene  
Concen: 1.950 ng  
RT: 13.79 min Scan# 1284  
Delta R.T. -0.00 min  
Lab File: BN007162.D  
Acq: 14 Aug 2019 10:33

Tgt Ion:152 Resp: 195404  
Ion Ratio Lower Upper  
152 100  
151 19.5 15.8 23.6  
153 13.6 10.4 15.6

