

#29

Benzo(a)anthracene

Concen: 10.302 ng

RT: 21.03 min Scan# 2170

Delta R.T. -0.00 min

Lab File: BN007162.D

Acq: 14 Aug 2019 10:33

Instrument :

BNA\_N

ClientSampled :


Tgt Ion:228 Resp: 1564210

Ion Ratio Lower Upper

228 100

226 32.4 21.8 32.6




229 22.8 15.6 23.4

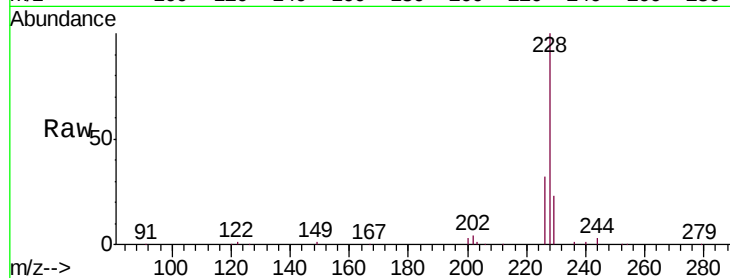

Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E

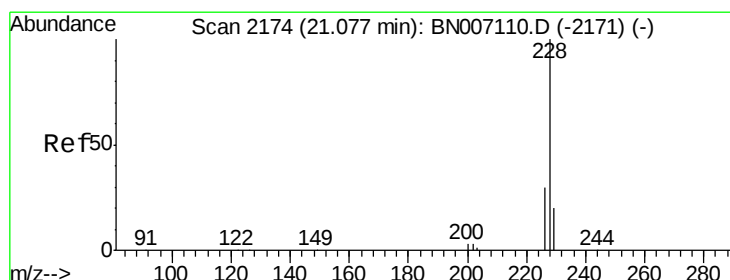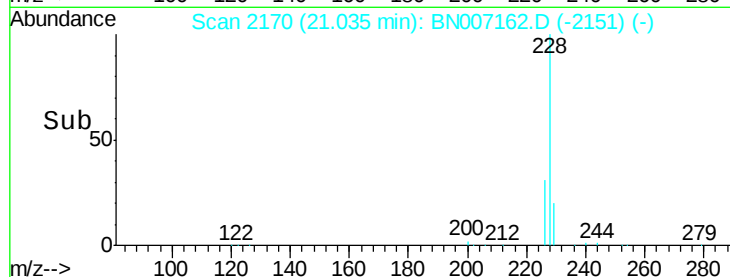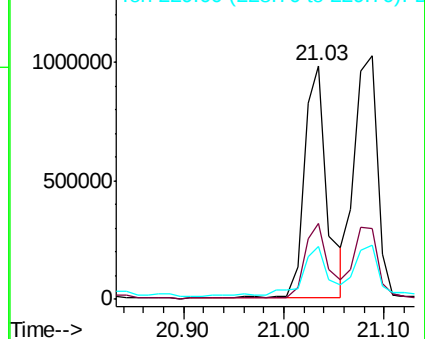

#30

Chrysene

Concen: 11.001 ng

RT: 21.09 min Scan# 2175

Delta R.T. -0.00 min

Lab File: BN007162.D

Acq: 14 Aug 2019 10:33


Tgt Ion:228 Resp: 1622883

Ion Ratio Lower Upper

228 100

226 29.0 23.8 35.6

229 22.0 15.7 23.5

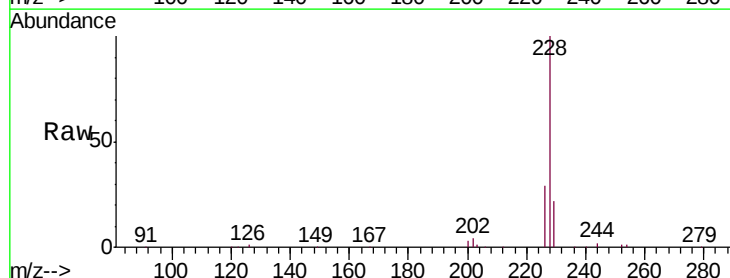

Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E

