

#33

Benzo(b)fluoranthene

Concen: 10.277 ng

RT: 22.54 min Scan# 2340

Delta R.T. -0.00 min

Lab File: BN007162.D

Acq: 14 Aug 2019 10:33

Instrument :

BNA_N

ClientSampleId :


Tgt Ion:252 Resp: 1821567

Ion Ratio Lower Upper




252 100

253 23.1 18.2 27.2

125 9.0 7.4 11.0

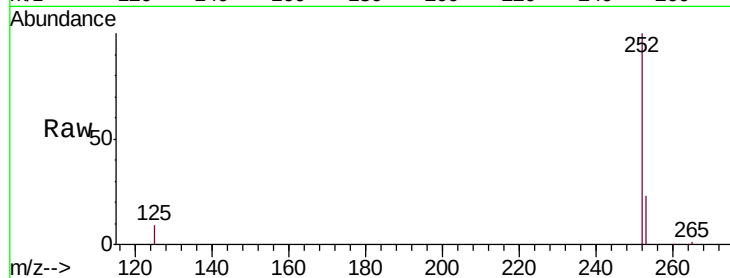

Abundance Ion 252.00 (251.70 to 252.70): E
Ion 253.00 (252.70 to 253.70): E
Ion 125.00 (124.70 to 125.70): E

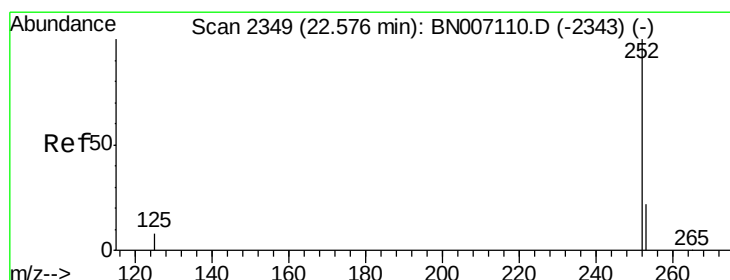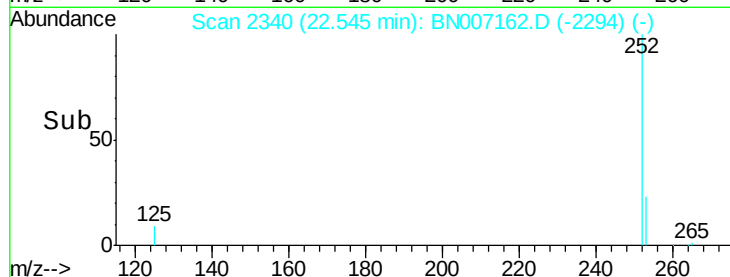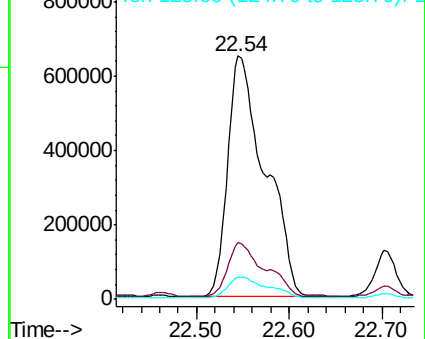

#34

Benzo(k)fluoranthene

Concen: 10.415 ng

RT: 22.54 min Scan# 2340

Delta R.T. -0.04 min

Lab File: BN007162.D

Acq: 14 Aug 2019 10:33


Tgt Ion:252 Resp: 1823227

Ion Ratio Lower Upper

252 100

253 23.1 18.1 27.1

125 9.0 7.4 11.0

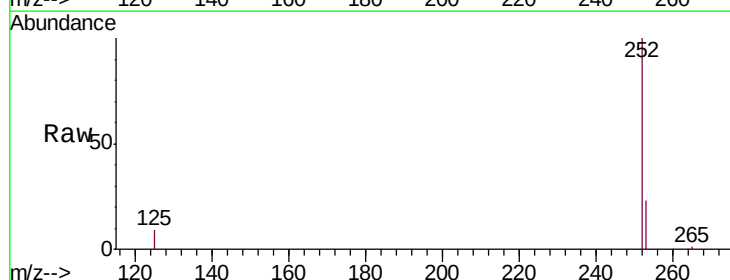

Abundance Ion 252.00 (251.70 to 252.70): E
Ion 253.00 (252.70 to 253.70): E
Ion 125.00 (124.70 to 125.70): E

