

#35

Benzo(a)pyrene

Concen: 7.413 ng

RT: 23.08 min Scan# 2495

Delta R.T. -0.01 min

Lab File: BN007162.D

Acq: 14 Aug 2019 10:33

Instrument :

BNA_N

ClientSampleId :





Tgt Ion:252 Resp: 1191231

Ion Ratio Lower Upper

252 100

253 23.0 18.5 27.7

125 9.2 8.2 12.4

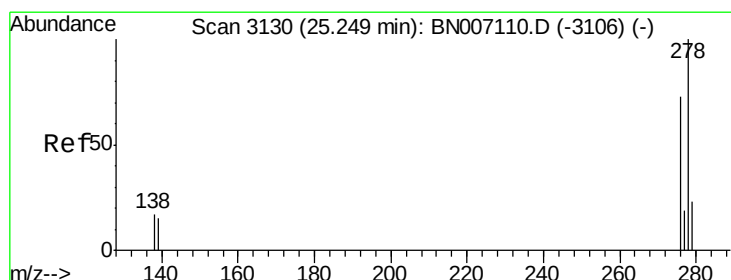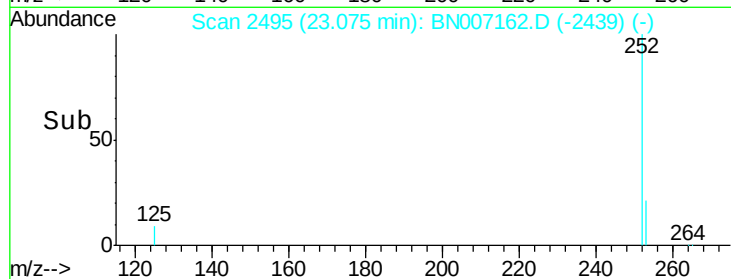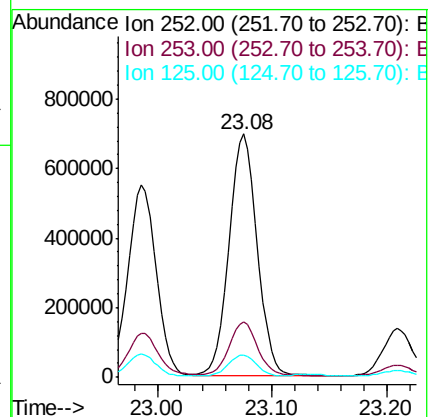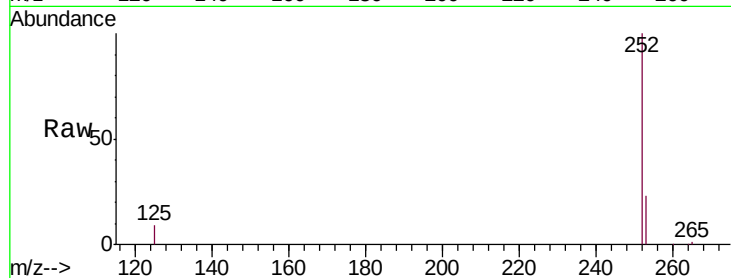

#36

Dibenzo(a,h)anthracene

Concen: 1.349 ng

RT: 25.25 min Scan# 3131

Delta R.T. -0.02 min

Lab File: BN007162.D

Acq: 14 Aug 2019 10:33

Tgt Ion:278 Resp: 216306

Ion Ratio Lower Upper

278 100

139 17.2 11.3 16.9#

279 29.4 19.3 28.9#

