

#6

Naphthalene-d8

Concen: 0.400 ng

RT: 10.19 min Scan# 813

Delta R.T. -0.00 min

Lab File: BN007163.D

Acq: 14 Aug 2019 11:09

Instrument :

BNA_N

ClientSampleId :

Tgt Ion:136 Resp: 35530


Ion Ratio Lower Upper

136 100

137 11.4 9.4 14.0

54 6.3 6.6 9.8#

68 5.9 6.0 9.0#



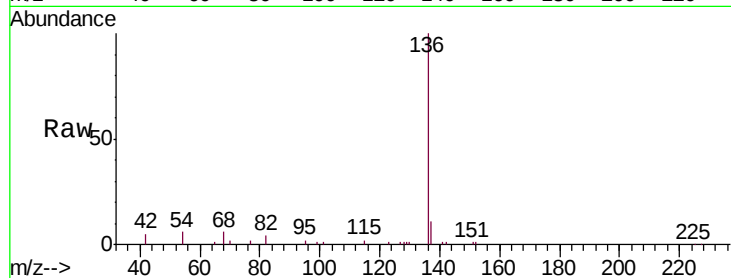


Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BNC

Ion 68.00 (67.70 to 68.70): BNC

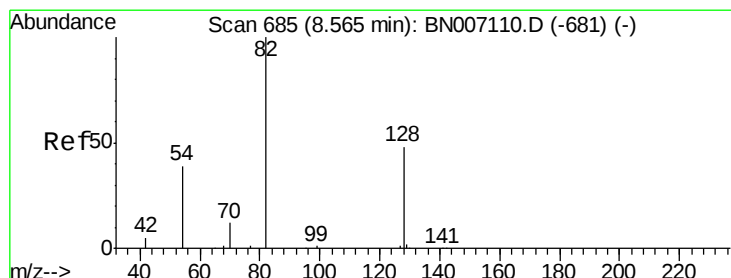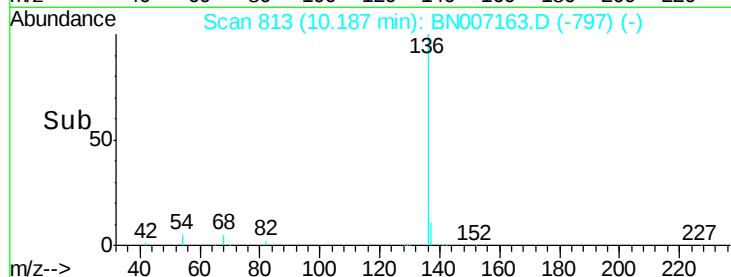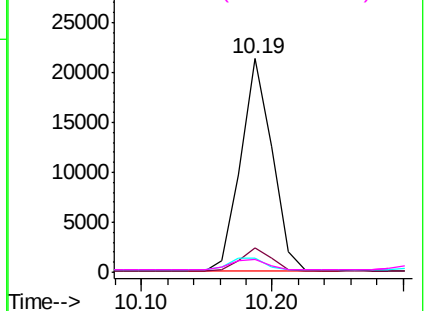

#7

Nitrobenzene-d5

Concen: 0.212 ng

RT: 8.56 min Scan# 685

Delta R.T. -0.00 min

Lab File: BN007163.D

Acq: 14 Aug 2019 11:09


Tgt Ion: 82 Resp: 6086

Ion Ratio Lower Upper

82 100

128 50.6 34.6 51.8

54 43.6 36.2 54.4

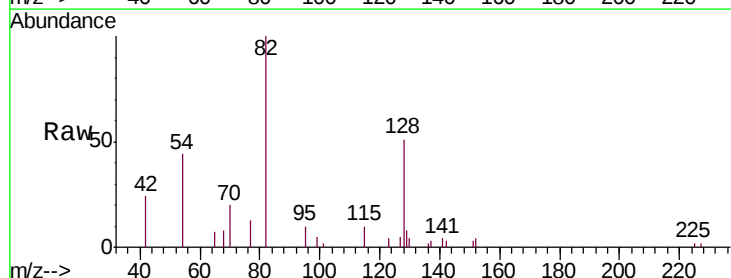

Abundance Ion 82.00 (81.70 to 82.70): BNC

Ion 128.00 (127.70 to 128.70): E

Ion 54.00 (53.70 to 54.70): BNC

