
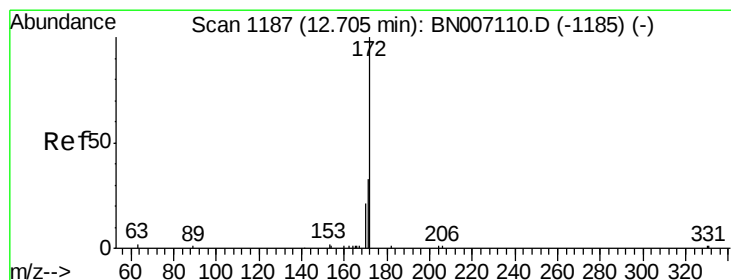
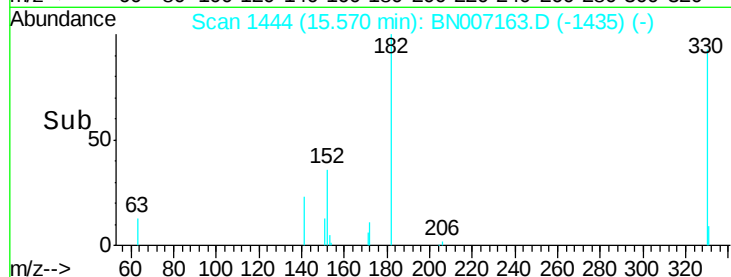
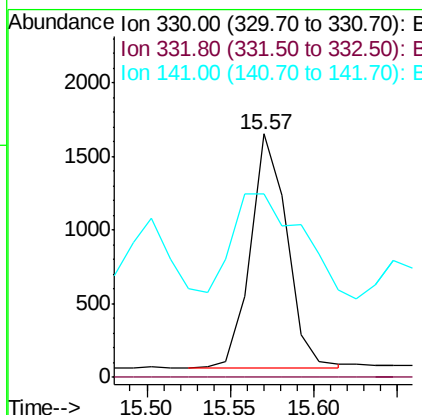


#13
 2,4,6-Tribromophenol
 Concen: 0.219 ng
 RT: 15.57 min Scan# 1444
 Delta R.T. -0.00 min
 Lab File: BN007163.D
 Acq: 14 Aug 2019 11:09

Instrument :
 BNA_N
 ClientSampleId :

Tgt Ion: 330 Resp: 2385
 Ion Ratio Lower Upper
 330 100
 332 0.0 0.0 0.0
 141 86.2 33.6 50.4#

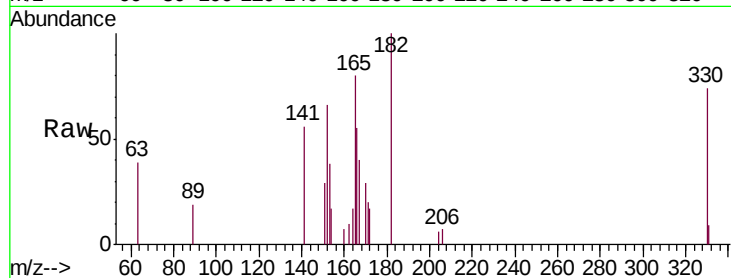

#14
 2-Fluorobiphenyl
 Concen: 0.121 ng
 RT: 12.71 min Scan# 1187
 Delta R.T. -0.00 min
 Lab File: BN007163.D
 Acq: 14 Aug 2019 11:09

Tgt Ion: 172 Resp: 3568
 Ion Ratio Lower Upper
 172 100
 171 32.6 26.3 39.5
 170 21.0 17.0 25.4

