
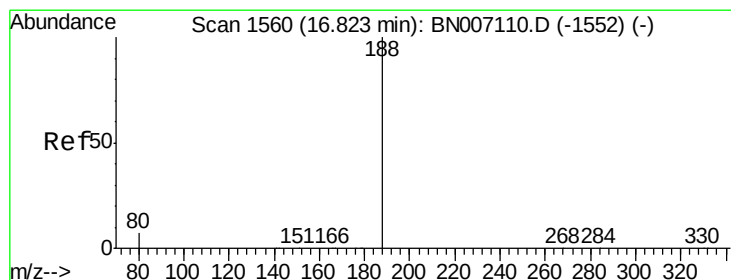
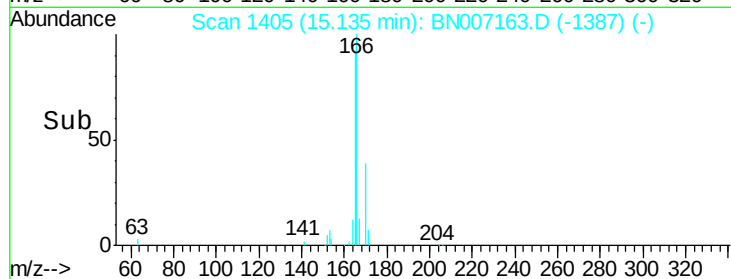
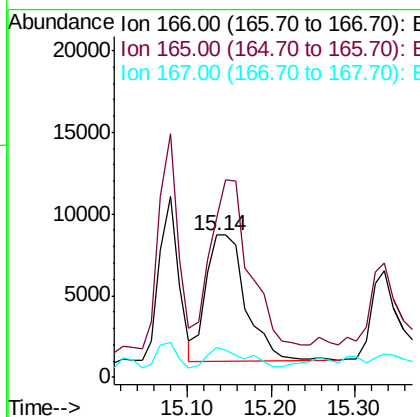


#17
 Fluorene
 Concen: 0.253 ng
 RT: 15.14 min Scan# 1405
 Delta R.T. -0.00 min
 Lab File: BN007163.D
 Acq: 14 Aug 2019 11:09

Instrument :
 BNA_N
 ClientSampleId :

Tgt Ion:166 Resp: 25636
 Ion Ratio Lower Upper
 166 100
 165 128.3 77.9 116.9#
 167 15.6 10.9 16.3

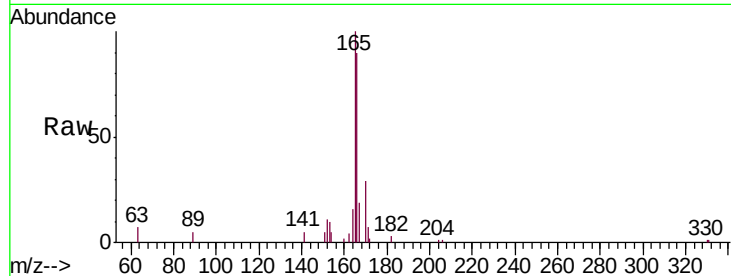

#18
 Phenanthrene-d10
 Concen: 0.400 ng
 RT: 16.82 min Scan# 1560
 Delta R.T. -0.00 min
 Lab File: BN007163.D
 Acq: 14 Aug 2019 11:09

Tgt Ion:188 Resp: 46156
 Ion Ratio Lower Upper
 188 100
 94 0.0 0.0 0.0
 80 9.1 7.8 11.6

