

#28

Terphenyl-d14

Concen: 0.226 ng

RT: 19.49 min Scan# 1969

Delta R.T. -0.01 min


Lab File: BN007163.D

Acq: 14 Aug 2019 11:09

Instrument :

BNA_N

ClientSampleId :

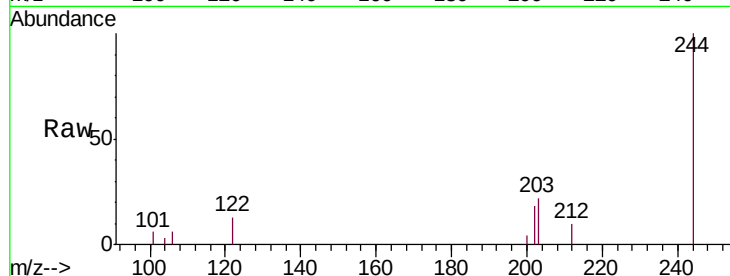




Tgt Ion:244 Resp: 26318

Ion Ratio Lower Upper

244 100

212 10.1 6.2 9.2#

122 12.9 7.4 11.2#

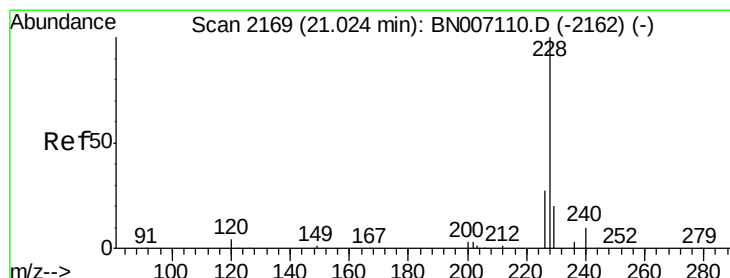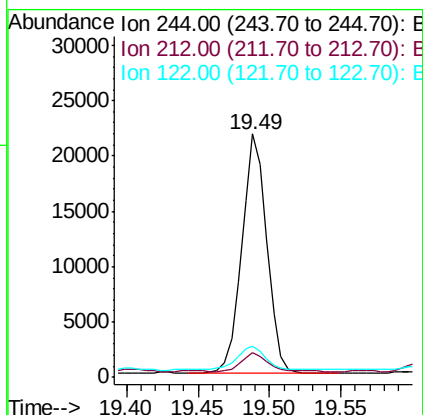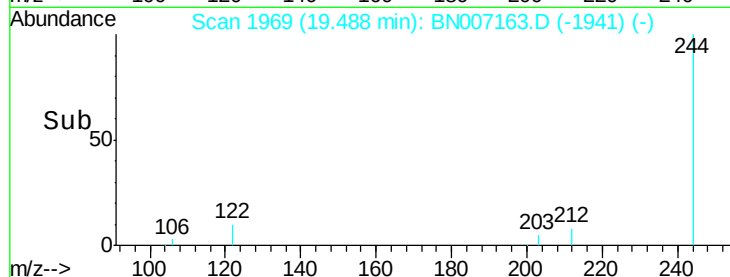

#29

Benzo(a)anthracene

Concen: 2.296 ng

RT: 21.08 min Scan# 2174

Delta R.T. 0.04 min

Lab File: BN007163.D

Acq: 14 Aug 2019 11:09

Tgt Ion:228 Resp: 358775

Ion Ratio Lower Upper

228 100

226 31.3 21.8 32.6

229 23.0 15.6 23.4

