
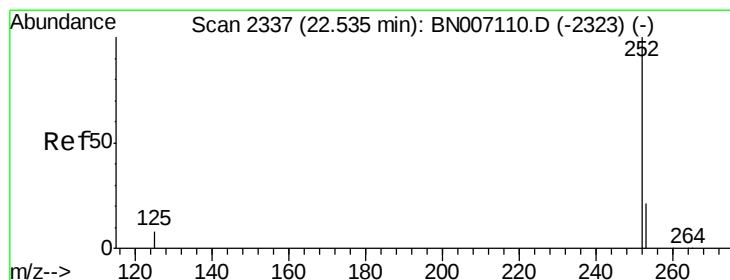
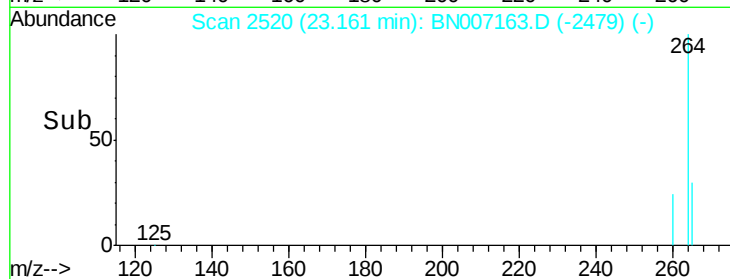
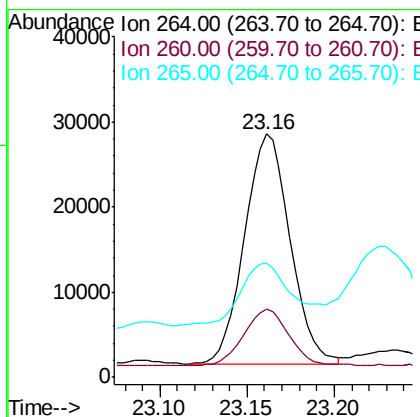


#32
 Perylene-d12
 Concen: 0.400 ng
 RT: 23.16 min Scan# 2520
 Delta R.T. -0.01 min
 Lab File: BN007163.D
 Acq: 14 Aug 2019 11:09

Instrument :
 BNA_N
 ClientSampleId :

Tgt Ion: 264 Resp: 49363
 Ion Ratio Lower Upper
 264 100
 260 27.8 19.8 29.8
 265 47.0 26.2 39.4#

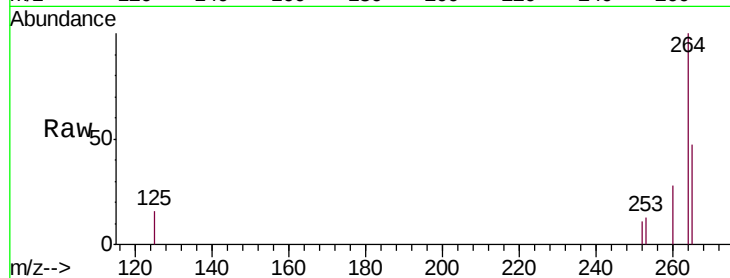

#33
 Benzo(b)fluoranthene
 Concen: 2.616 ng
 RT: 22.54 min Scan# 2339
 Delta R.T. -0.01 min
 Lab File: BN007163.D
 Acq: 14 Aug 2019 11:09

Tgt Ion: 252 Resp: 442866
 Ion Ratio Lower Upper
 252 100
 253 23.5 18.2 27.2
 125 10.7 7.4 11.0

