

#34

Benzo(k)fluoranthene

Concen: 2.649 ng

RT: 22.54 min Scan# 2339

Delta R.T. -0.05 min

Lab File: BN007163.D

Acq: 14 Aug 2019 11:09

Instrument :

BNA_N

ClientSampled :


Tgt Ion:252 Resp: 442866

Ion Ratio Lower Upper

252 100

253 23.5 18.1 27.1




125 10.7 7.4 11.0

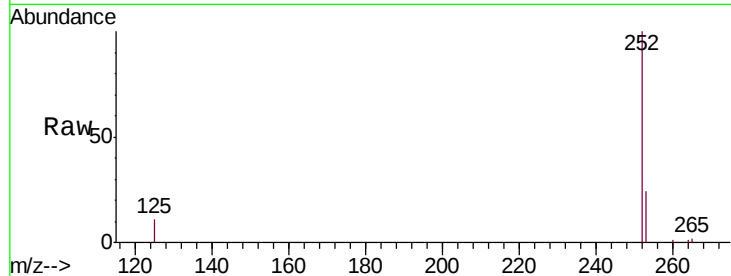

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

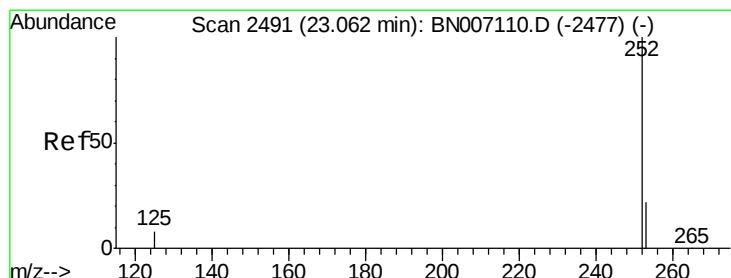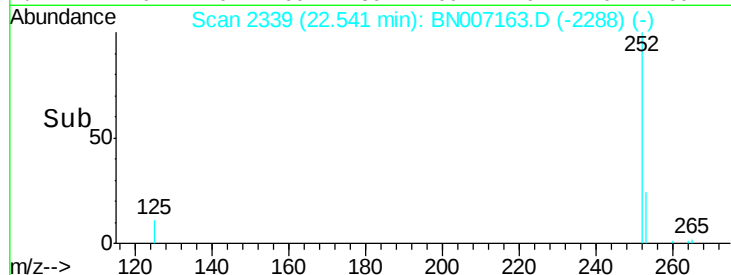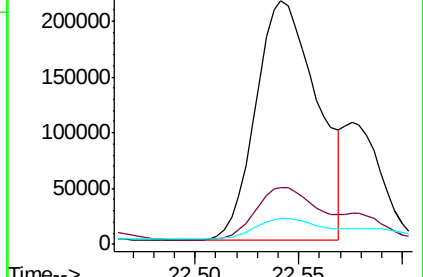

#35

Benzo(a)pyrene

Concen: 2.088 ng

RT: 23.07 min Scan# 2493

Delta R.T. -0.01 min

Lab File: BN007163.D

Acq: 14 Aug 2019 11:09


Tgt Ion:252 Resp: 320446

Ion Ratio Lower Upper

252 100

253 23.8 18.5 27.7

125 11.4 8.2 12.4

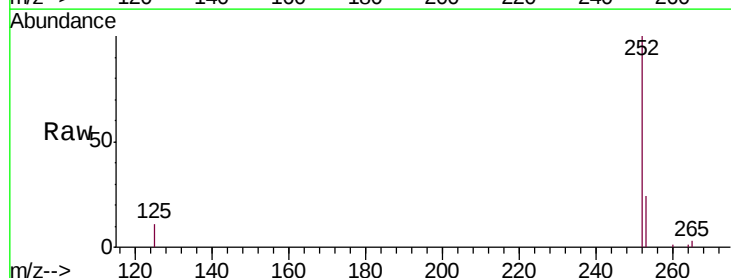

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

