

#36

Dibenzo(a,h)anthracene

Concen: 0.420 ng

RT: 25.25 min Scan# 3131

Delta R.T. -0.02 min


Lab File: BN007163.D

Acq: 14 Aug 2019 11:09

Instrument :

BNA_N

ClientSampleId :

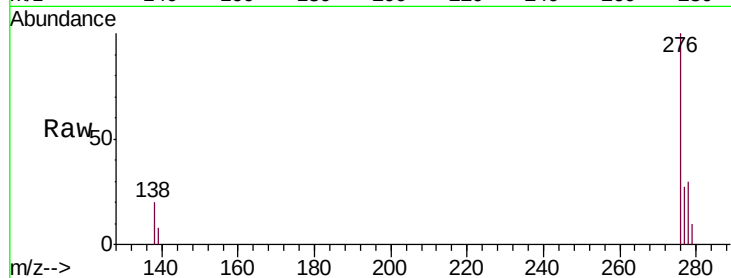




Tgt Ion:278 Resp: 64264

Ion Ratio Lower Upper

278 100

139 25.9 11.3 16.9#

279 33.6 19.3 28.9#

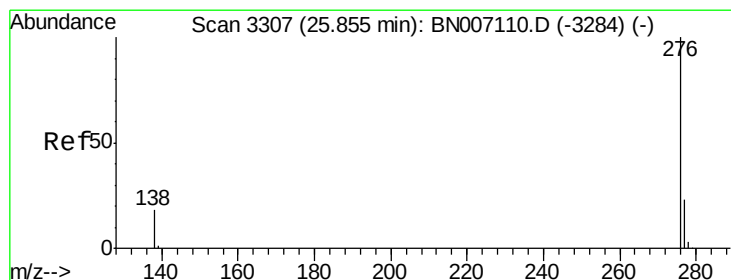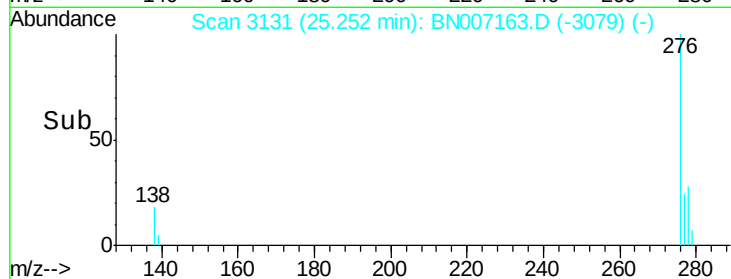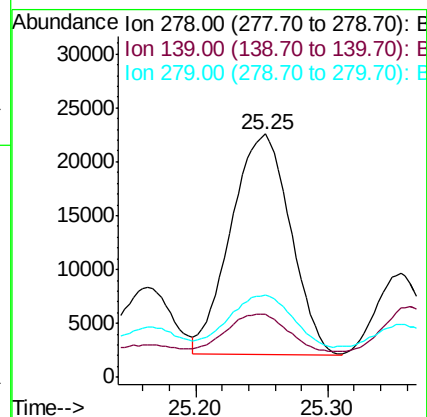

#37

Benzo(g,h,i)perylene

Concen: 1.669 ng

RT: 25.87 min Scan# 3312

Delta R.T. -0.01 min

Lab File: BN007163.D

Acq: 14 Aug 2019 11:09

Tgt Ion:276 Resp: 262851

Ion Ratio Lower Upper

276 100

277 25.2 19.8 29.8

138 19.8 14.6 22.0

