

#16

Acenaphthene

Concen: 0.450 ng

RT: 14.14 min Scan# 1316

Delta R.T. -0.00 min

Lab File: BN007164.D

Acq: 14 Aug 2019 11:45

Instrument :

BNA_N

ClientSampled :


Tgt Ion:154 Resp: 31331

Ion Ratio Lower Upper

154 100

153 119.7 89.5 134.3




152 54.3 44.8 67.2

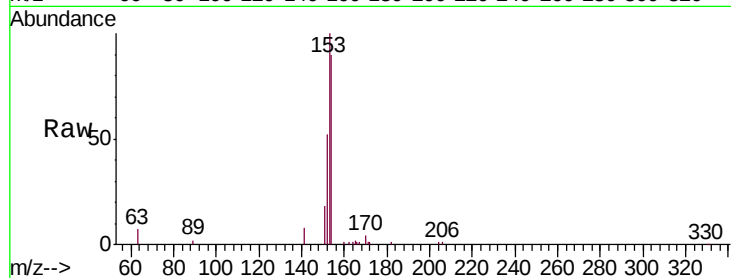

Abundance Ion 154.00 (153.70 to 154.70): E

Ion 153.00 (152.70 to 153.70): E

Ion 152.00 (151.70 to 152.70): E

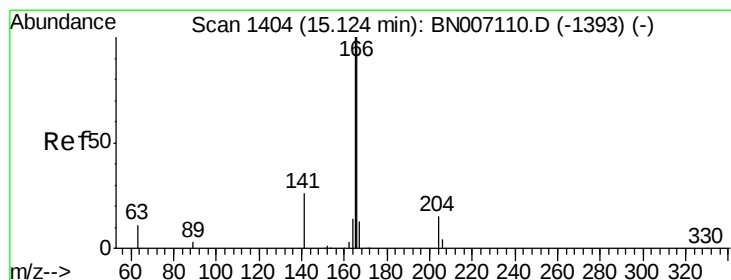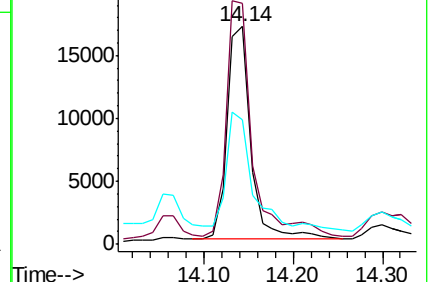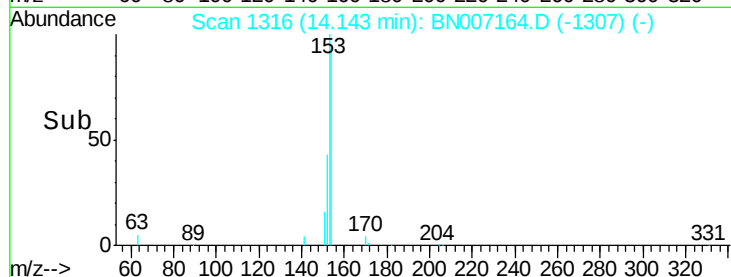

#17

Fluorene

Concen: 0.769 ng

RT: 15.13 min Scan# 1405

Delta R.T. -0.00 min

Lab File: BN007164.D

Acq: 14 Aug 2019 11:45


Tgt Ion:166 Resp: 80098

Ion Ratio Lower Upper

166 100

165 113.6 77.9 116.9

167 14.9 10.9 16.3

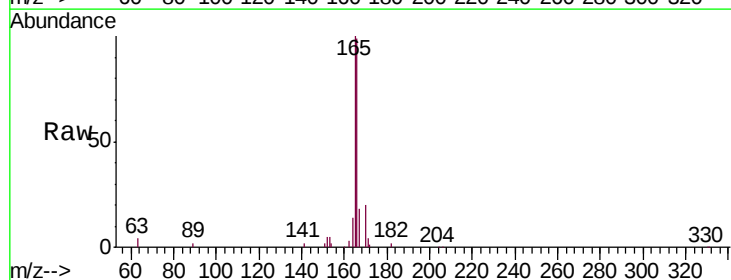

Abundance Ion 166.00 (165.70 to 166.70): E

Ion 165.00 (164.70 to 165.70): E

Ion 167.00 (166.70 to 167.70): E

