
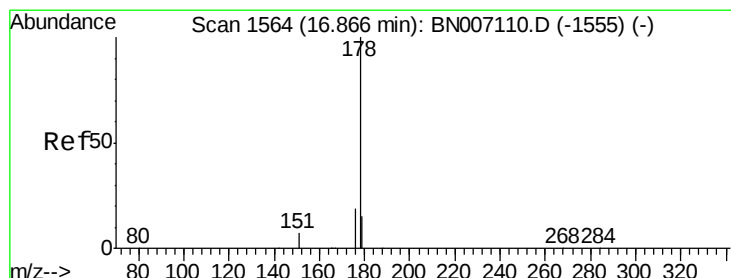
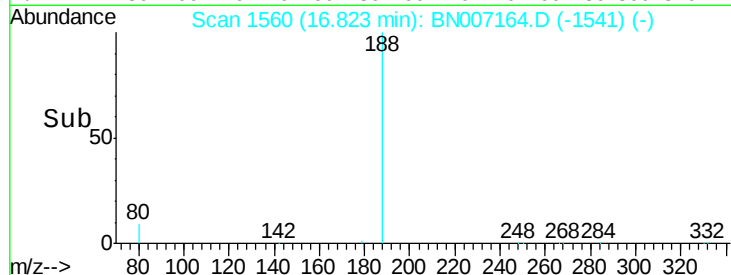
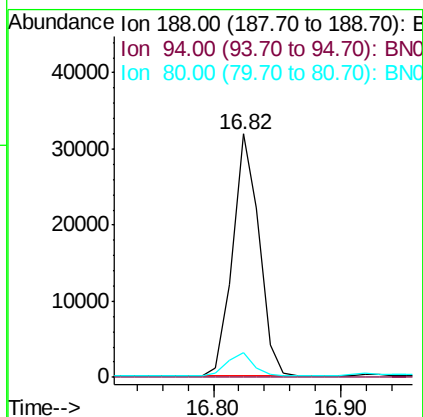


#18
Phenanthrene-d10
Concen: 0.400 ng
RT: 16.82 min Scan# 1560
Delta R.T. -0.00 min
Lab File: BN007164.D
Acq: 14 Aug 2019 11:45

Instrument :
BNA_N
ClientSampleId :

Tgt Ion:188 Resp: 45633
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 9.9 7.8 11.6

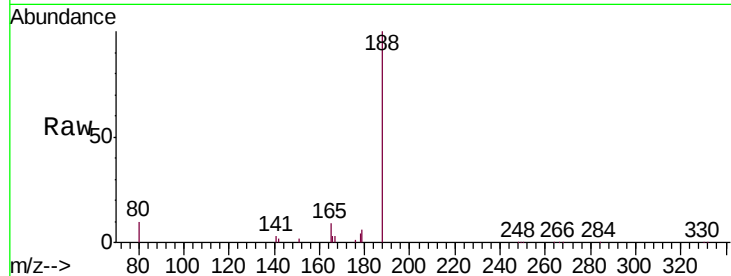

#22
Phenanthrene
Concen: 9.734 ng
RT: 16.87 min Scan# 1564
Delta R.T. -0.00 min
Lab File: BN007164.D
Acq: 14 Aug 2019 11:45

Tgt Ion:178 Resp: 1331259
Ion Ratio Lower Upper
178 100
176 18.9 15.2 22.8
179 15.7 12.3 18.5

