

#23

Anthracene

Concen: 2.173 ng

RT: 16.96 min Scan# 1573

Delta R.T. -0.00 min

Lab File: BN007164.D

Acq: 14 Aug 2019 11:45

Instrument :

BNA_N

ClientSampleId :


Tgt Ion:178 Resp: 271468

Ion Ratio Lower Upper

178 100

176 18.2 14.6 21.8




179 16.5 12.5 18.7

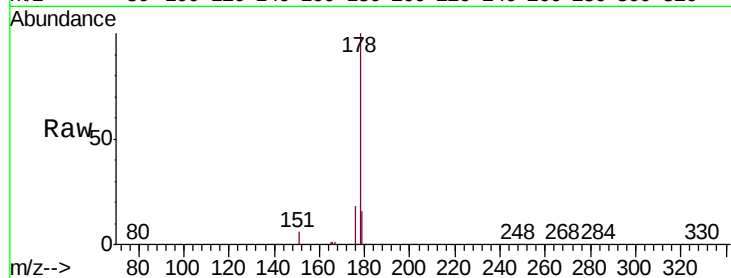

Abundance Ion 178.00 (177.70 to 178.70): E

Ion 176.00 (175.70 to 176.70): E

Ion 179.00 (178.70 to 179.70): E

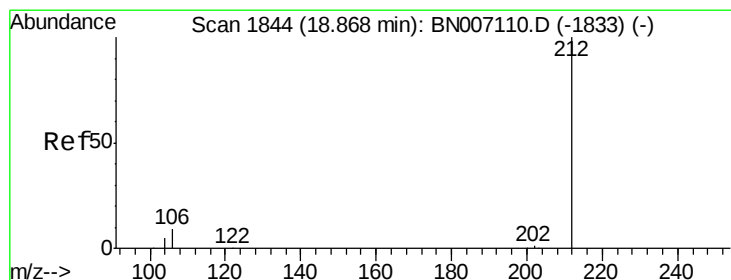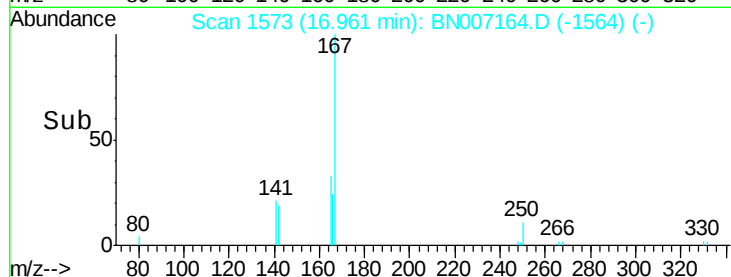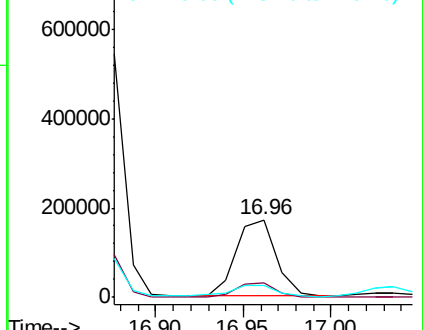

#24

Fluoranthene-d10

Concen: 0.025 ng

RT: 18.79 min Scan# 1828

Delta R.T. -0.08 min

Lab File: BN007164.D

Acq: 14 Aug 2019 11:45


Tgt Ion:212 Resp: 4000

Ion Ratio Lower Upper

212 100

106 10.7 8.2 12.2

104 6.5 4.5 6.7

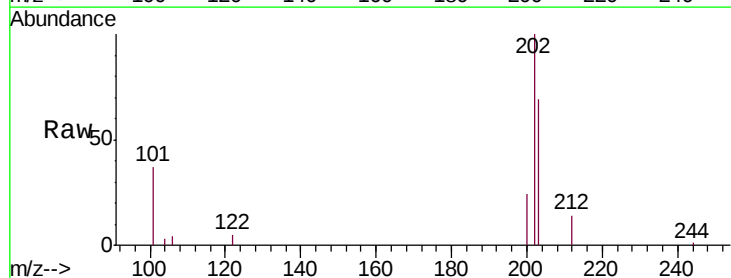

Abundance Ion 212.00 (211.70 to 212.70): E

Ion 106.00 (105.70 to 106.70): E

Ion 104.00 (103.70 to 104.70): E

