

#29

Benzo(a)anthracene

Concen: 5.548 ng

RT: 21.08 min Scan# 2174

Delta R.T. 0.04 min

Lab File: BN007164.D

Acq: 14 Aug 2019 11:45

Instrument :

BNA_N

ClientSampleId :





Tgt Ion:228 Resp: 890731

Ion Ratio Lower Upper

228 100

226 31.4 21.8 32.6

229 22.1 15.6 23.4

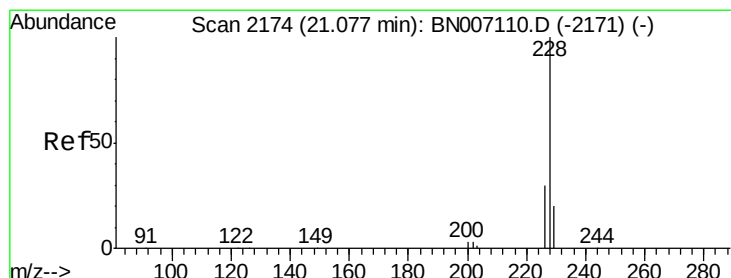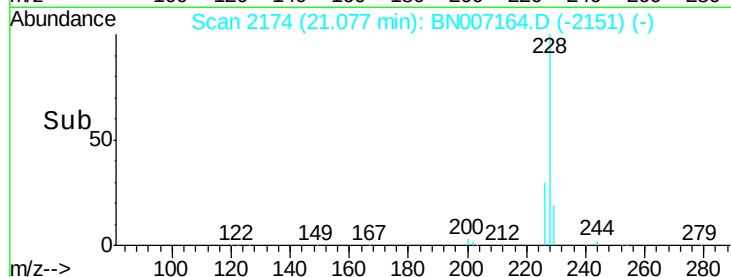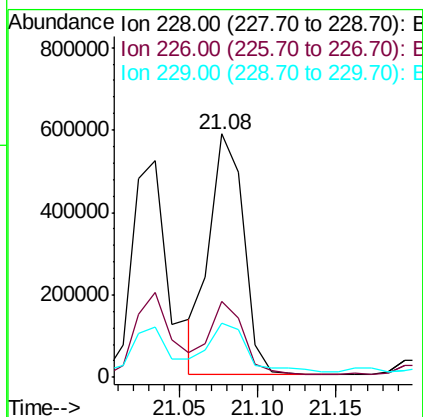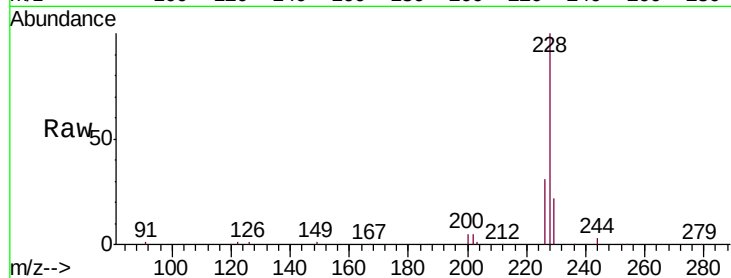

#30

Chrysene

Concen: 5.708 ng

RT: 21.08 min Scan# 2174

Delta R.T. -0.01 min

Lab File: BN007164.D

Acq: 14 Aug 2019 11:45

Tgt Ion:228 Resp: 890364

Ion Ratio Lower Upper

228 100

226 31.4 23.8 35.6

229 22.1 15.7 23.5

