

#35

Benzo(a)pyrene

Concen: 4.296 ng

RT: 23.07 min Scan# 2494

Delta R.T. -0.01 min

Lab File: BN007164.D

Acq: 14 Aug 2019 11:45

Instrument :

BNA\_N

ClientSampled :


Tgt Ion:252 Resp: 692112

Ion Ratio Lower Upper




252 100

253 22.9 18.5 27.7

125 9.7 8.2 12.4

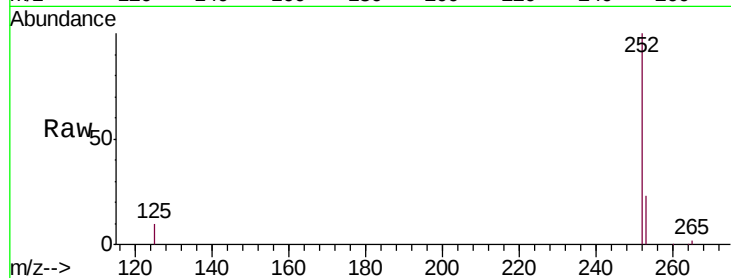

Abundance Ion 252.00 (251.70 to 252.70): E  
Ion 253.00 (252.70 to 253.70): E  
Ion 125.00 (124.70 to 125.70): E

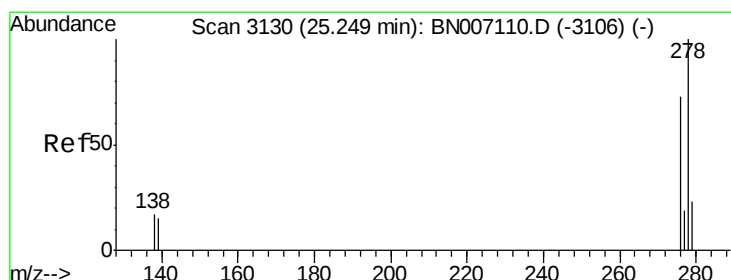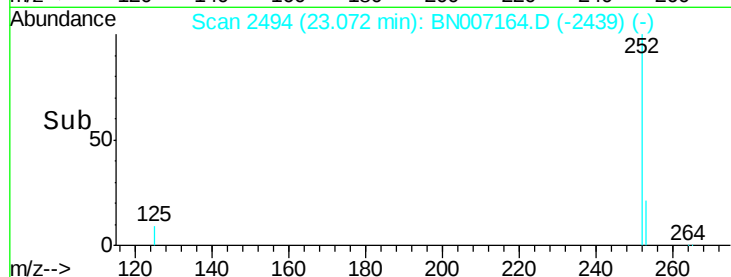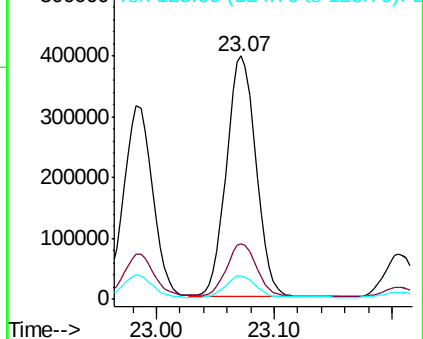

#36

Dibenzo(a,h)anthracene

Concen: 0.778 ng

RT: 25.26 min Scan# 3132

Delta R.T. -0.02 min

Lab File: BN007164.D

Acq: 14 Aug 2019 11:45


Tgt Ion:278 Resp: 125069

Ion Ratio Lower Upper

278 100

139 19.2 11.3 16.9#

279 32.0 19.3 28.9#

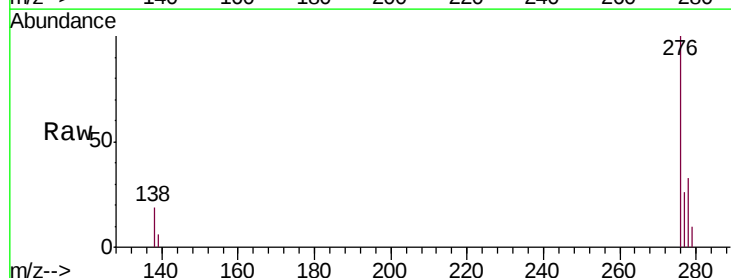

Abundance Ion 278.00 (277.70 to 278.70): E  
Ion 139.00 (138.70 to 139.70): E  
Ion 279.00 (278.70 to 279.70): E

