

#23

Anthracene

Concen: 2.466 ng

RT: 16.96 min Scan# 1573

Delta R.T. -0.00 min

Lab File: BN007165.D

Acq: 14 Aug 2019 12:21

Instrument :

BNA_N

ClientSampleId :





Tgt Ion:178 Resp: 319878

Ion Ratio Lower Upper

178 100

176 18.3 14.6 21.8

179 16.8 12.5 18.7

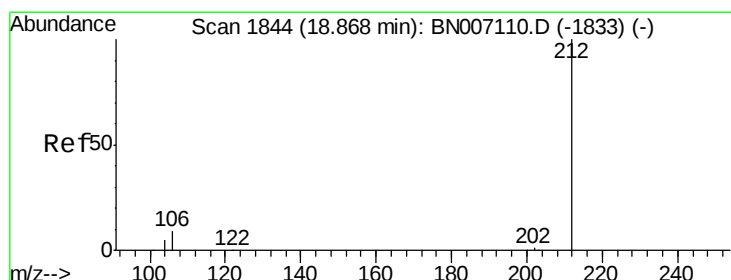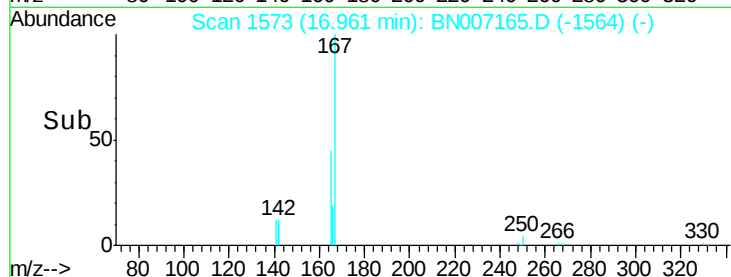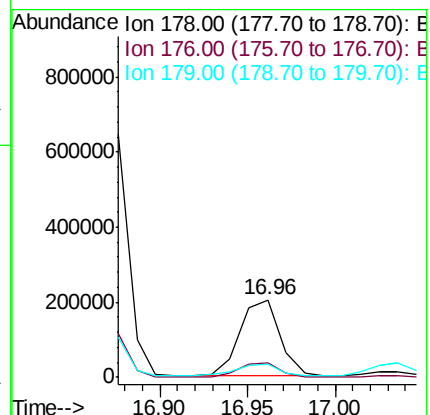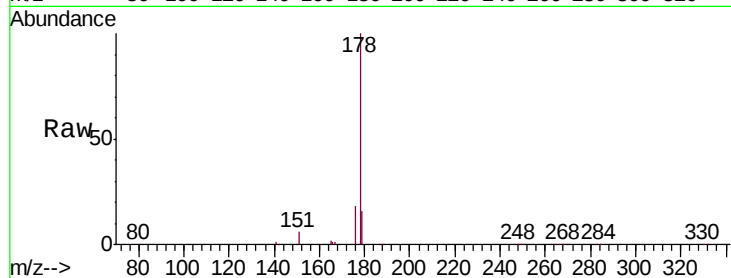

#24

Fluoranthene-d10

Concen: 0.042 ng

RT: 18.79 min Scan# 1828

Delta R.T. -0.08 min

Lab File: BN007165.D

Acq: 14 Aug 2019 12:21

Tgt Ion:212 Resp: 7120

Ion Ratio Lower Upper

212 100

106 11.9 8.2 12.2

104 6.3 4.5 6.7

