

#25

Fluoranthene

Concen: 13.018 ng

RT: 18.90 min Scan# 1851

Delta R.T. -0.00 min

Lab File: BN007165.D

Acq: 14 Aug 2019 12:21

Instrument :

BNA_N

ClientSampleId :


Tgt Ion:202 Resp: 2364319

Ion Ratio Lower Upper

202 100

101 9.0 7.0 10.4




203 18.1 13.8 20.8

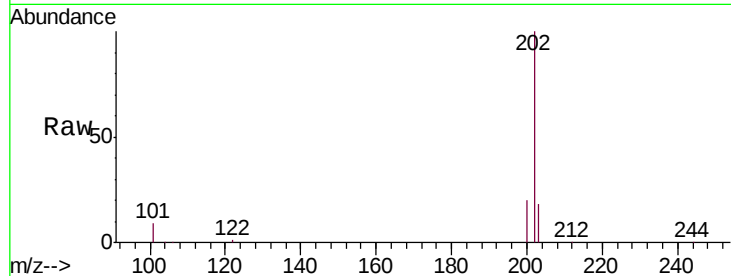

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 203.00 (202.70 to 203.70): E

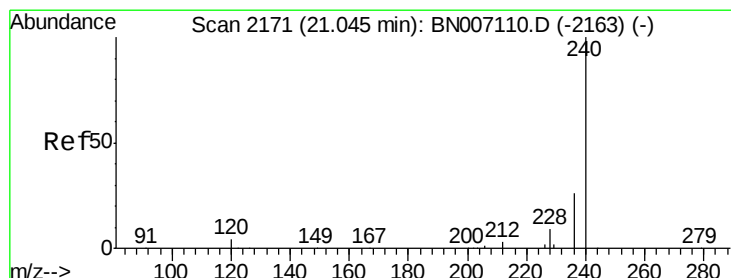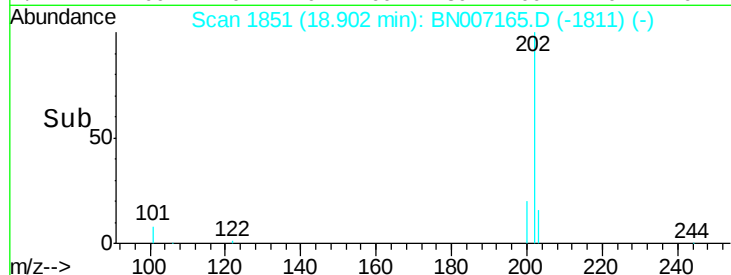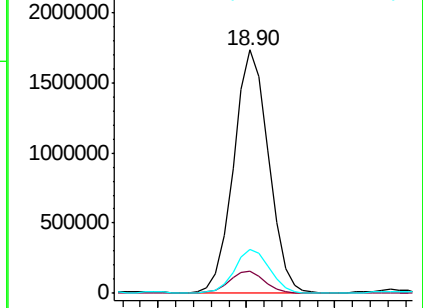

#26

Chrysene-d12

Concen: 0.400 ng

RT: 21.04 min Scan# 2171

Delta R.T. -0.01 min

Lab File: BN007165.D

Acq: 14 Aug 2019 12:21


Tgt Ion:240 Resp: 47522

Ion Ratio Lower Upper

240 100

120 16.5 4.0 6.0#

236 33.6 21.3 31.9#

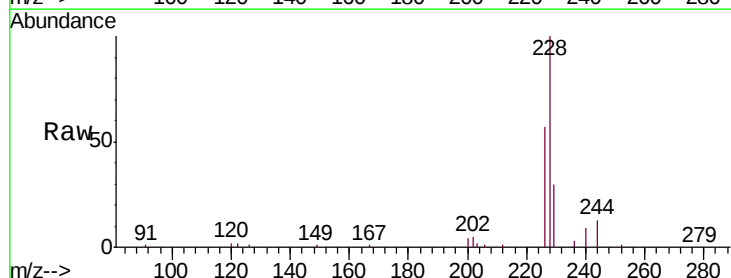

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

