

#35

Benzo(a)pyrene

Concen: 7.798 ng

RT: 23.08 min Scan# 2496

Delta R.T. -0.00 min

Lab File: BN007165.D

Acq: 14 Aug 2019 12:21

Instrument :

BNA_N

ClientSampleId :


Tgt Ion:252 Resp: 1382646

Ion Ratio Lower Upper




252 100

253 22.9 18.5 27.7

125 9.2 8.2 12.4

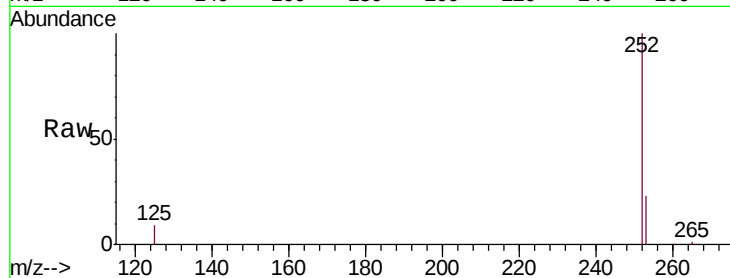

Abundance Ion 252.00 (251.70 to 252.70): E
Ion 253.00 (252.70 to 253.70): E
Ion 125.00 (124.70 to 125.70): E

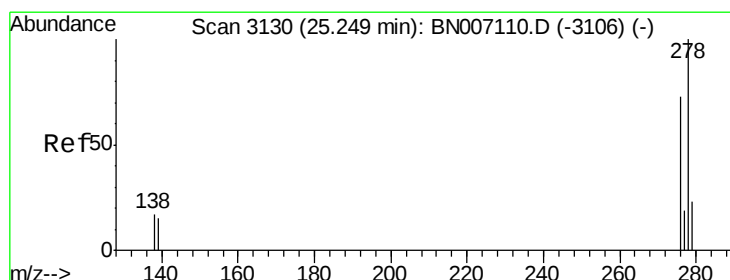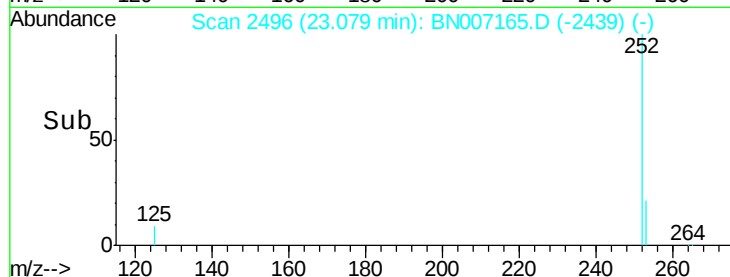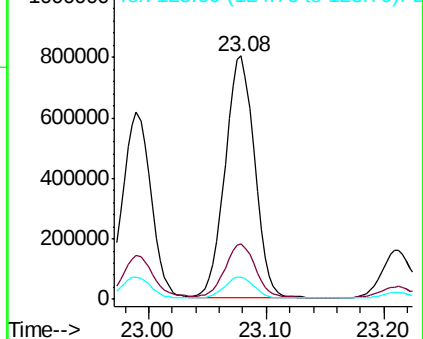

#36

Dibenzo(a,h)anthracene

Concen: 1.437 ng

RT: 25.26 min Scan# 3132

Delta R.T. -0.02 min

Lab File: BN007165.D

Acq: 14 Aug 2019 12:21


Tgt Ion:278 Resp: 254292

Ion Ratio Lower Upper

278 100

139 16.9 11.3 16.9

279 30.4 19.3 28.9#

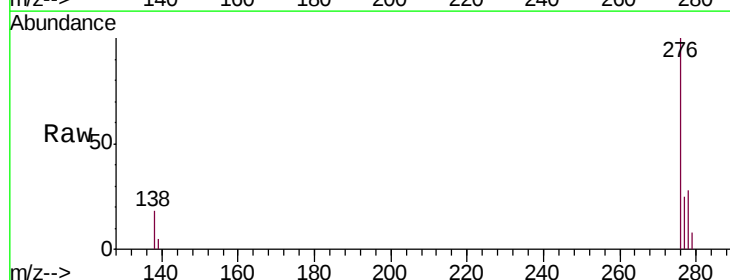

Abundance Ion 278.00 (277.70 to 278.70): E
Ion 139.00 (138.70 to 139.70): E
Ion 279.00 (278.70 to 279.70): E

