


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN081319\
 Data File : BN007129.D
 Acq On : 13 Aug 2019 13:31
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN081019.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Aug 13 12:12:02 2019

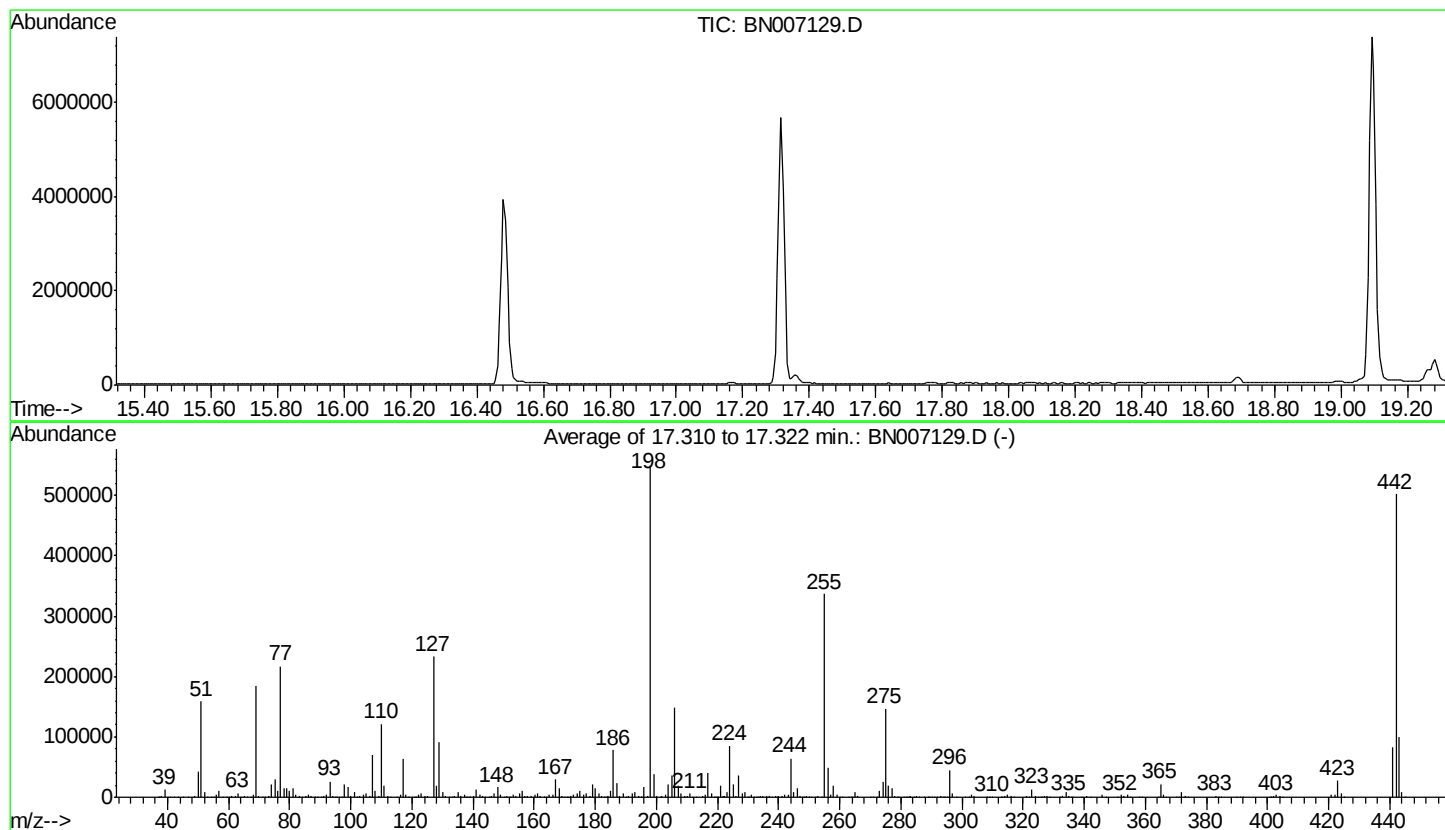

AutoFind: Scans 2435, 2436, 2437; Background Corrected with Scan 2428

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.8	158240	PASS
68	69	0.00	2	2.0	3707	PASS
69	198	0.00	100	33.6	184720	PASS
70	69	0.00	2	0.7	1291	PASS
127	198	10	80	42.4	233237	PASS
197	198	0.00	2	0.2	1174	PASS
198	198	100	100	100.0	549440	PASS
199	198	5	9	6.9	37944	PASS
275	198	10	60	26.6	146410	PASS
365	198	1	100	4.0	21778	PASS
441	198	0.01	100	15.2	83245	PASS
442	198	50	100	91.4	502378	PASS
443	442	15	24	19.8	99386	PASS