


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN081319\
 Data File : BN007148.D
 Acq On : 14 Aug 2019 01:32
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN081019.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Aug 13 12:12:02 2019

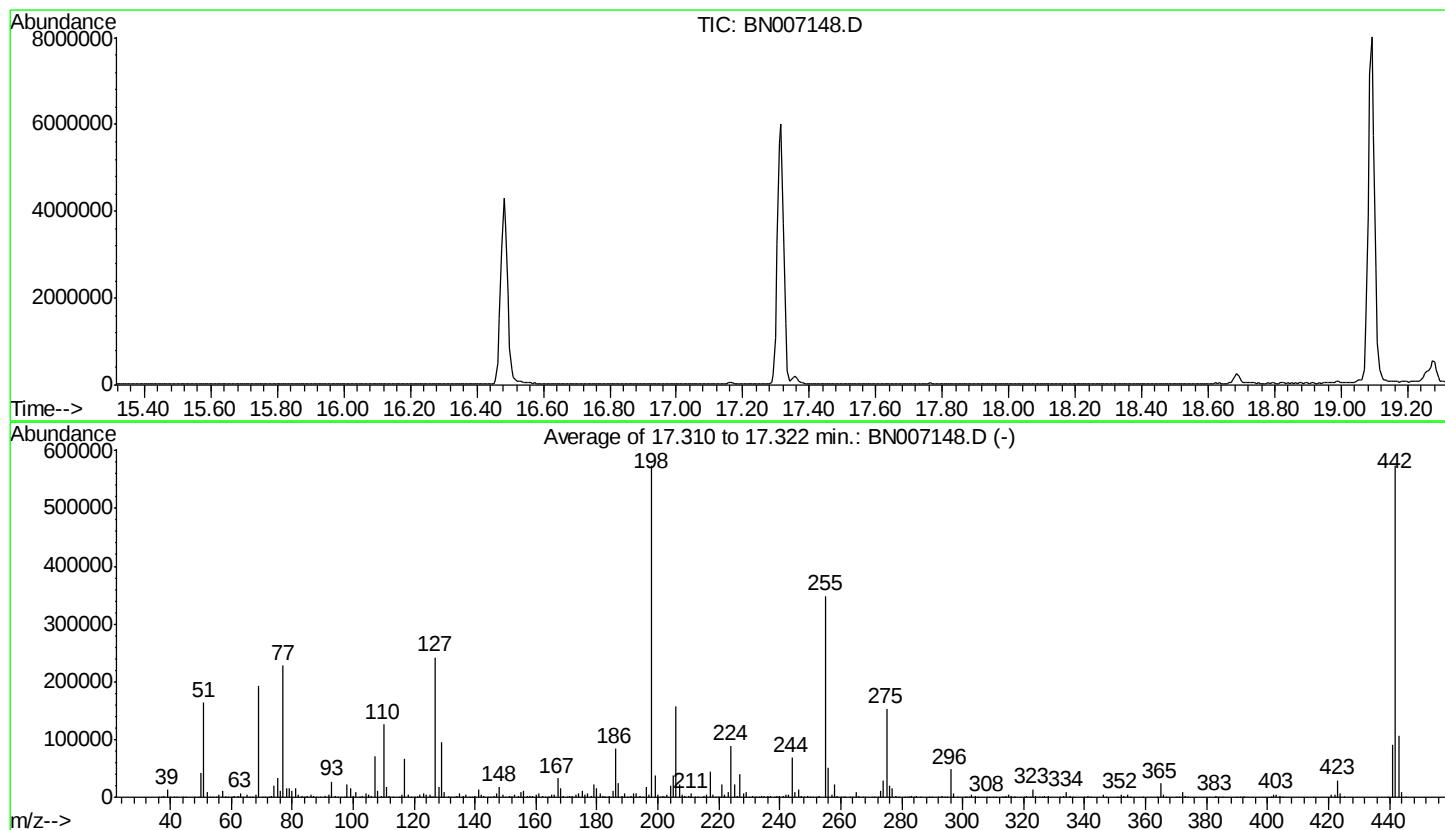

AutoFind: Scans 2435, 2436, 2437; Background Corrected with Scan 2428

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.5	163498	PASS
68	69	0.00	2	1.8	3469	PASS
69	198	0.00	100	33.5	192037	PASS
70	69	0.00	2	0.6	1121	PASS
127	198	10	80	42.2	242154	PASS
197	198	0.00	2	0.8	4338	PASS
198	198	100	100	100.0	574016	PASS
199	198	5	9	6.6	37813	PASS
275	198	10	60	26.8	153560	PASS
365	198	1	100	4.2	24274	PASS
441	198	0.01	100	15.7	89936	PASS
442	198	50	100	99.9	573440	PASS
443	442	15	24	18.7	107077	PASS