

Data File : BN007168.D
Acq On : 14 Aug 2019 18:04
Operator : HP/JU
Sample : SSTDCCC0.4
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

Quant Time: Aug 15 11:13:31 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN081019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 13 12:12:02 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.43	152	5906	0.40	ng	0.00
6) Naphthalene-d8	10.19	136	22011	0.40	ng	0.00
12) Acenaphthene-d10	14.08	164	13240	0.40	ng	0.00
18) Phenanthrene-d10	16.82	188	33762	0.40	ng	0.00
26) Chrysene-d12	21.05	240	34600	0.40	ng	-0.01
32) Perylene-d12	23.16	264	39106	0.40	ng	-0.01

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 2-Fluorophenol	5.05	112	6290	0.44	ng	0.00
4) Phenol-d6	6.61	99	7617	0.43	ng	0.00
7) Nitrobenzene-d5	8.55	82	7832	0.44	ng	-0.01
10) 2-Methylnaphthalene-d10	11.79	152	16102	0.39	ng	0.00
13) 2,4,6-Tribromophenol	15.57	330	3126	0.44	ng	0.00
14) 2-Fluorobiphenyl	12.71	172	2616	0.14	ng	0.00
24) Fluoranthene-d10	18.87	212	50697	0.42	ng	0.00
28) Terphenyl-d14	19.49	244	44066	0.47	ng	-0.01


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
2) n-Nitrosodimethylamine	3.34	42	1588	0.409	ng	# 97
5) bis(2-Chloroethyl)ether	6.86	93	6367	0.410	ng	99
8) Naphthalene	10.24	128	23973	0.388	ng	99
9) Hexachlorobutadiene	10.54	225	5389	0.410	ng	# 98
11) 2-Methylnaphthalene	11.86	142	17322	0.396	ng	97
15) Acenaphthylene	13.79	152	29550	0.427	ng	99
16) Acenaphthene	14.13	154	18076	0.408	ng	99
17) Fluorene	15.12	166	25156	0.379	ng	99
19) 4-Bromophenyl-phenylether	16.03	248	9136	0.438	ng	# 92
20) Hexachlorobenzene	16.14	284	8700	0.433	ng	99
21) Pentachlorophenol	16.48	266	3498	0.467	ng	97
22) Phenanthrene	16.87	178	43694	0.432	ng	100
23) Anthracene	16.95	178	41069	0.444	ng	99
25) Fluoranthene	18.90	202	55425	0.428	ng	100
27) Pyrene	19.26	202	57012	0.470	ng	100
29) Benzo(a)anthracene	21.02	228	57290	0.453	ng	99
30) Chrysene	21.08	228	54404	0.443	ng	99
31) Indeno(1,2,3-cd)pyrene	25.24	276	66923	0.494	ng	98
33) Benzo(b)fluoranthene	22.53	252	58797	0.438	ng	97
34) Benzo(k)fluoranthene	22.58	252	56490m	0.427	ng	
35) Benzo(a)pyrene	23.07	252	53971	0.444	ng	# 97
36) Dibenzo(a,h)anthracene	25.25	278	54442	0.449	ng	# 96
37) Benzo(g,h,i)perylene	25.86	276	54427	0.436	ng	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BN007168.D
Acq On : 14 Aug 2019 18:04
Operator : HP/JU
Sample : SSTDCCC0.4
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

Quant Time: Aug 15 11:13:31 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN081019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 13 12:12:02 2019
Response via : Initial Calibration






#1




1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 7.43 min Scan# 546
Delta R.T. -0.01 min
Lab File: BN007168.D
Acq: 14 Aug 2019 18:04

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

Tgt Ion: 152 Resp: 5906
Ion Ratio Lower Upper
152 100
150 151.4 121.7 182.5
115 60.4 46.2 69.4




Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

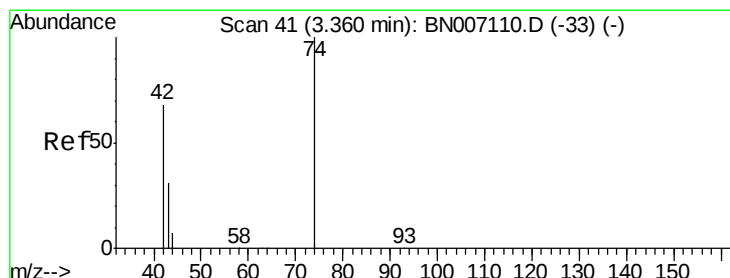



#2


n-Nitrosodimethylamine
Concen: 0.409 ng
RT: 3.34 min Scan# 39
Delta R.T. -0.02 min
Lab File: BN007168.D
Acq: 14 Aug 2019 18:04

Tgt Ion: 42 Resp: 1588
Ion Ratio Lower Upper
42 100
74 141.7 110.6 166.0
44 17.7 0.0 0.0#



Abundance Ion 42.00 (41.70 to 42.70): BNC
Ion 74.00 (73.70 to 74.70): BNC
Ion 44.00 (43.70 to 44.70): BNC





#3

2-Fluorophenol

Concen: 0.443 ng

RT: 5.05 min Scan# 251

Delta R.T. -0.01 min

Lab File: BN007168.D

Acq: 14 Aug 2019 18:04

Instrument :

BNA_N

ClientSampleId :

SSTDCCC0.4


Tgt Ion: 112 Resp: 6290

Ion Ratio Lower Upper

112 100

64 51.3 42.6 63.8




63 27.9 22.2 33.2



Abundance Ion 112.00 (111.70 to 112.70): BNC

Ion 64.00 (63.70 to 64.70): BNC

Ion 63.00 (62.70 to 63.70): BNC



#4

Phenol-d6

Concen: 0.433 ng

RT: 6.61 min Scan# 445

Delta R.T. -0.00 min

Lab File: BN007168.D

Acq: 14 Aug 2019 18:04


Tgt Ion: 99 Resp: 7617

Ion Ratio Lower Upper

99 100

42 18.5 15.8 23.6



71 34.8 27.0 40.4




Abundance Ion 99.00 (98.70 to 99.70): BNC

Ion 42.00 (41.70 to 42.70): BNC

Ion 71.00 (70.70 to 71.70): BNC









#5

bis(2-Chloroethyl)ether
Concen: 0.410 ng
RT: 6.86 min Scan# 476
Delta R.T. -0.01 min
Lab File: BN007168.D
Acq: 14 Aug 2019 18:04

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4




Tgt Ion:	93	Resp:	6367
Ion	Ratio	Lower	Upper
93	100		
63	68.7	55.6	83.4
95	32.7	26.7	40.1




#6

Naphthalene-d8
Concen: 0.400 ng
RT: 10.19 min Scan# 813
Delta R.T. -0.00 min
Lab File: BN007168.D
Acq: 14 Aug 2019 18:04

Tgt Ion:	136	Resp:	22011
Ion	Ratio	Lower	Upper
136	100		
137	11.5	9.4	14.0
54	5.5	6.6	9.8#
68	5.3	6.0	9.0#





#7

Nitrobenzene-d5

Concen: 0.441 ng

RT: 8.55 min Scan# 684

Delta R.T. -0.01 min

Lab File: BN007168.D

Acq: 14 Aug 2019 18:04

Instrument :

BNA_N

ClientSampleId :

SSTDCCC0.4


Tgt Ion: 82 Resp: 7832

Ion Ratio Lower Upper

82 100

128 40.2 34.6 51.8




54 48.8 36.2 54.4



Abundance Ion 82.00 (81.70 to 82.70): BN0

Ion 128.00 (127.70 to 128.70): BN0

Ion 54.00 (53.70 to 54.70): BN0



#8

Naphthalene

Concen: 0.388 ng

RT: 10.24 min Scan# 817

Delta R.T. -0.00 min

Lab File: BN007168.D

Acq: 14 Aug 2019 18:04


Tgt Ion: 128 Resp: 23973

Ion Ratio Lower Upper

128 100

129 12.2 9.4 14.2



127 13.6 11.0 16.6




Abundance Ion 128.00 (127.70 to 128.70): BN0

Ion 129.00 (128.70 to 129.70): BN0

Ion 127.00 (126.70 to 127.70): BN0





#9

Hexachlorobutadiene

Concen: 0.410 ng

RT: 10.54 min Scan# 841

Delta R.T. -0.01 min

Lab File: BN007168.D

Acq: 14 Aug 2019 18:04

Instrument :

BNA_N

ClientSampleId :

SSTDCCC0.4


Tgt Ion:225 Resp: 5389

Ion Ratio Lower Upper

225 100

223 0.0 0.0 0.0




227 65.3 51.1 76.7



Abundance Ion 225.00 (224.70 to 225.70): E

Ion 223.00 (222.70 to 223.70): E

Ion 227.00 (226.70 to 227.70): E



#10

2-Methylnaphthalene-d10

Concen: 0.392 ng

RT: 11.79 min Scan# 980

Delta R.T. -0.01 min

Lab File: BN007168.D


Acq: 14 Aug 2019 18:04

Tgt Ion:152 Resp: 16102

Ion Ratio Lower Upper



152 100


151 19.4 15.5 23.3



Abundance Ion 152.00 (151.70 to 152.70): E

Ion 151.00 (150.70 to 151.70): E





#11

2-Methylnaphthalene

Concen: 0.396 ng

RT: 11.86 min Scan# 997

Delta R.T. -0.01 min

Lab File: BN007168.D

Acq: 14 Aug 2019 18:04

Instrument :

BNA_N

ClientSampleId :

SSTDCCC0.4


Tgt Ion:142 Resp: 17322

Ion Ratio Lower Upper




142 100

141 89.6 69.0 103.6

115 35.1 27.1 40.7



Abundance Ion 142.00 (141.70 to 142.70): E
Ion 141.00 (140.70 to 141.70): E
Ion 115.00 (114.70 to 115.70): E



#12

Acenaphthene-d10

Concen: 0.400 ng

RT: 14.08 min Scan# 1310

Delta R.T. -0.00 min

Lab File: BN007168.D

Acq: 14 Aug 2019 18:04


Tgt Ion:164 Resp: 13240

Ion Ratio Lower Upper



164 100


162 100.2 82.2 123.4

160 45.8 38.3 57.5



Abundance Ion 164.00 (163.70 to 164.70): E
Ion 162.00 (161.70 to 162.70): E
Ion 160.00 (159.70 to 160.70): E









#13
 2,4,6-Tribromophenol
 Concen: 0.438 ng
 RT: 15.57 min Scan# 1444
 Delta R.T. -0.00 min
 Lab File: BN007168.D
 Acq: 14 Aug 2019 18:04




Instrument :
 BNA_N
 ClientSampleId :
 SSTDCCC0.4


Tgt Ion: 330 Resp: 3126
 Ion Ratio Lower Upper
 330 100
 332 0.0 0.0 0.0
 141 41.0 33.6 50.4



#14
 2-Fluorobiphenyl
 Concen: 0.136 ng
 RT: 12.71 min Scan# 1187
 Delta R.T. -0.00 min
 Lab File: BN007168.D
 Acq: 14 Aug 2019 18:04

Tgt Ion: 172 Resp: 2616
 Ion Ratio Lower Upper
 172 100
 171 32.6 26.3 39.5
 170 21.5 17.0 25.4





#15

Acenaphthylene

Concen: 0.427 ng

RT: 13.79 min Scan# 1284

Delta R.T. -0.00 min

Lab File: BN007168.D

Acq: 14 Aug 2019 18:04

Instrument :

BNA_N

ClientSampleId :

SSTDCCC0.4


Tgt Ion:152 Resp: 29550

Ion Ratio Lower Upper

152 100

151 19.4 15.8 23.6




153 13.2 10.4 15.6



Abundance Ion 152.00 (151.70 to 152.70): E

Ion 151.00 (150.70 to 151.70): E

Ion 153.00 (152.70 to 153.70): E



#16

Acenaphthene

Concen: 0.408 ng

RT: 14.13 min Scan# 1315

Delta R.T. -0.01 min

Lab File: BN007168.D

Acq: 14 Aug 2019 18:04


Tgt Ion:154 Resp: 18076

Ion Ratio Lower Upper

154 100

153 111.3 89.5 134.3



152 54.5 44.8 67.2




Abundance Ion 154.00 (153.70 to 154.70): E

Ion 153.00 (152.70 to 153.70): E

Ion 152.00 (151.70 to 152.70): E





#17

Fluorene

Concen: 0.379 ng

RT: 15.12 min Scan# 1404

Delta R.T. -0.01 min

Lab File: BN007168.D

Acq: 14 Aug 2019 18:04

Instrument :

BNA_N

ClientSampleId :

SSTDCCC0.4


Tgt Ion:166 Resp: 25156

Ion Ratio Lower Upper

166 100

165 96.4 77.9 116.9




167 13.4 10.9 16.3



Abundance Ion 166.00 (165.70 to 166.70): E

Ion 165.00 (164.70 to 165.70): E

Ion 167.00 (166.70 to 167.70): E



#18

Phenanthrene-d10

Concen: 0.400 ng

RT: 16.82 min Scan# 1560

Delta R.T. -0.00 min

Lab File: BN007168.D

Acq: 14 Aug 2019 18:04


Tgt Ion:188 Resp: 33762

Ion Ratio Lower Upper

188 100

94 0.0 0.0 0.0



80 7.5 7.8 11.6#




Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BNC

Ion 80.00 (79.70 to 80.70): BNC





#19

4-Bromophenyl-phenylether

Concen: 0.438 ng

RT: 16.03 min Scan# 1485

Delta R.T. -0.01 min

Lab File: BN007168.D

Acq: 14 Aug 2019 18:04

Instrument :

BNA_N

ClientSampleId :

SSTDCCC0.4


Tgt Ion:248 Resp: 9136

Ion Ratio Lower Upper

248 100

250 96.1 78.9 118.3




141 67.4 43.3 64.9#



Abundance Ion 248.00 (247.70 to 248.70): E

Ion 250.00 (249.70 to 250.70): E

Ion 141.00 (140.70 to 141.70): E



#20

Hexachlorobenzene

Concen: 0.433 ng

RT: 16.14 min Scan# 1496

Delta R.T. -0.00 min

Lab File: BN007168.D

Acq: 14 Aug 2019 18:04


Tgt Ion:284 Resp: 8700

Ion Ratio Lower Upper

284 100

142 36.7 30.5 45.7



249 33.4 26.7 40.1




Abundance Ion 283.80 (283.50 to 284.50): E

Ion 142.00 (141.70 to 142.70): E

Ion 249.00 (248.70 to 249.70): E





#21

Pentachlorophenol

Concen: 0.467 ng

RT: 16.48 min Scan# 1528

Delta R.T. -0.00 min

Lab File: BN007168.D

Acq: 14 Aug 2019 18:04

Instrument :

BNA_N

ClientSampleId :

SSTDCCC0.4


Tgt Ion:266 Resp: 3498

Ion Ratio Lower Upper

266 100

264 62.3 52.3 78.5




268 65.2 51.5 77.3



Abundance Ion 266.00 (265.70 to 266.70): E

Ion 264.00 (263.70 to 264.70): E

Ion 268.00 (267.70 to 268.70): E



#22

Phenanthrene

Concen: 0.432 ng

RT: 16.87 min Scan# 1564

Delta R.T. -0.00 min

Lab File: BN007168.D

Acq: 14 Aug 2019 18:04


Tgt Ion:178 Resp: 43694

Ion Ratio Lower Upper

178 100

176 19.4 15.2 22.8



179 15.4 12.3 18.5




Abundance Ion 178.00 (177.70 to 178.70): E

Ion 176.00 (175.70 to 176.70): E

Ion 179.00 (178.70 to 179.70): E





#23

Anthracene

Concen: 0.444 ng

RT: 16.95 min Scan# 1572

Delta R.T. -0.01 min

Lab File: BN007168.D

Acq: 14 Aug 2019 18:04

Instrument :

BNA_N

ClientSampleId :

SSTDCCC0.4





Tgt Ion:178 Resp: 41069

Ion Ratio Lower Upper

178 100

176 18.4 14.6 21.8

179 15.1 12.5 18.7



#24

Fluoranthene-d10

Concen: 0.423 ng

RT: 18.87 min Scan# 1844

Delta R.T. -0.01 min

Lab File: BN007168.D

Acq: 14 Aug 2019 18:04




Tgt Ion:212 Resp: 50697


Ion Ratio Lower Upper

212 100

106 10.5 8.2 12.2

104 5.7 4.5 6.7





#25

Fluoranthene

Concen: 0.428 ng

RT: 18.90 min Scan# 1850

Delta R.T. -0.01 min

Lab File: BN007168.D

Acq: 14 Aug 2019 18:04

Instrument :

BNA_N

ClientSampleId :

SSTDCCC0.4


Tgt Ion:202 Resp: 55425

Ion Ratio Lower Upper

202 100

101 9.2 7.0 10.4




203 17.3 13.8 20.8



Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 203.00 (202.70 to 203.70): E



#26

Chrysene-d12

Concen: 0.400 ng

RT: 21.05 min Scan# 2171

Delta R.T. -0.01 min

Lab File: BN007168.D

Acq: 14 Aug 2019 18:04


Tgt Ion:240 Resp: 34600

Ion Ratio Lower Upper

240 100

120 6.1 4.0 6.0#



236 26.8 21.3 31.9




Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E









#27
 Pyrene
 Concen: 0.470 ng
 RT: 19.26 min Scan# 1924
 Delta R.T. -0.01 min
 Lab File: BN007168.D
 Acq: 14 Aug 2019 18:04




Instrument :
 BNA_N
 ClientSampleId :
 SSTDCCC0.4


Tgt Ion: 202 Resp: 57012
 Ion Ratio Lower Upper
 202 100
 200 20.8 16.6 24.8
 203 17.7 14.0 21.0



#28
 Terphenyl-d14
 Concen: 0.467 ng
 RT: 19.49 min Scan# 1969
 Delta R.T. -0.01 min
 Lab File: BN007168.D
 Acq: 14 Aug 2019 18:04

Tgt Ion: 244 Resp: 44066
 Ion Ratio Lower Upper
 244 100
 212 7.8 6.2 9.2
 122 9.8 7.4 11.2





#29

Benzo(a)anthracene

Concen: 0.453 ng

RT: 21.02 min Scan# 2169

Delta R.T. -0.01 min

Lab File: BN007168.D

Acq: 14 Aug 2019 18:04

Instrument :

BNA_N

ClientSampleId :

SSTDCCC0.4


Tgt Ion:228 Resp: 57290

Ion Ratio Lower Upper

228 100

226 27.7 21.8 32.6




229 20.0 15.6 23.4



Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E



#30

Chrysene

Concen: 0.443 ng

RT: 21.08 min Scan# 2174

Delta R.T. -0.01 min

Lab File: BN007168.D

Acq: 14 Aug 2019 18:04


Tgt Ion:228 Resp: 54404

Ion Ratio Lower Upper

228 100

226 30.2 23.8 35.6



229 19.8 15.7 23.5




Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E





#31

Indeno(1,2,3-cd)pyrene

Concen: 0.494 ng

RT: 25.24 min Scan# 3127

Delta R.T. -0.01 min

Lab File: BN007168.D

Acq: 14 Aug 2019 18:04

Instrument :

BNA_N

ClientSampleId :

SSTDCCC0.4


Tgt Ion:276 Resp: 66923

Ion Ratio Lower Upper

276 100

138 21.8 16.0 24.0




277 25.1 19.9 29.9



Abundance Ion 276.00 (275.70 to 276.70): E

Ion 138.00 (137.70 to 138.70): E

Ion 277.00 (276.70 to 277.70): E



#32

Perylene-d12

Concen: 0.400 ng

RT: 23.16 min Scan# 2520

Delta R.T. -0.01 min

Lab File: BN007168.D

Acq: 14 Aug 2019 18:04


Tgt Ion:264 Resp: 39106

Ion Ratio Lower Upper

264 100

260 24.6 19.8 29.8



265 34.8 26.2 39.4




Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E





#33

Benzo(b)fluoranthene

Concen: 0.438 ng

RT: 22.53 min Scan# 2337

Delta R.T. -0.01 min

Lab File: BN007168.D

Acq: 14 Aug 2019 18:04

Instrument :

BNA_N

ClientSampleId :

SSTDCCC0.4


Tgt Ion:252 Resp: 58797

Ion Ratio Lower Upper

252 100

253 23.5 18.2 27.2




125 10.9 7.4 11.0



Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E



#34

Benzo(k)fluoranthene

Concen: 0.427 ng m

RT: 22.58 min Scan# 2349

Delta R.T. -0.01 min

Lab File: BN007168.D

Acq: 14 Aug 2019 18:04


Tgt Ion:252 Resp: 56490

Ion Ratio Lower Upper

252 100

253 23.5 18.1 27.1



125 12.3 7.4 11.0#




Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E





#35

Benzo(a)pyrene

Concen: 0.444 ng

RT: 23.07 min Scan# 2492

Delta R.T. -0.02 min

Lab File: BN007168.D

Acq: 14 Aug 2019 18:04

Instrument :

BNA_N

ClientSampleId :

SSTDCCC0.4


Tgt Ion:252 Resp: 53971

Ion Ratio Lower Upper

252 100

253 23.9 18.5 27.7




125 12.4 8.2 12.4#



Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E



#36

Dibenzo(a,h)anthracene

Concen: 0.449 ng

RT: 25.25 min Scan# 3131

Delta R.T. -0.02 min

Lab File: BN007168.D

Acq: 14 Aug 2019 18:04


Tgt Ion:278 Resp: 54442

Ion Ratio Lower Upper

278 100

139 17.5 11.3 16.9#



279 24.6 19.3 28.9




Abundance Ion 278.00 (277.70 to 278.70): E

Ion 139.00 (138.70 to 139.70): E

Ion 279.00 (278.70 to 279.70): E





#37

Benzo(g,h,i)perylene

Concen: 0.436 ng

RT: 25.86 min Scan# 3309

Delta R.T. -0.02 min

Lab File: BN007168.D


Acq: 14 Aug 2019 18:04

Instrument :

BNA_N

ClientSampleId :

SSTDCCC0.4




Tgt Ion: 276 Resp: 54427

Ion Ratio Lower Upper

276 100

277 25.2 19.8 29.8

138 20.2 14.6 22.0



Abundance

Ion 276.00 (275.70 to 276.70): E

Ion 277.00 (276.70 to 277.70): E

Ion 138.00 (137.70 to 138.70): E

