


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN081419\
 Data File : BN007167.D
 Acq On : 14 Aug 2019 17:28
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN081019.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Aug 13 12:12:02 2019

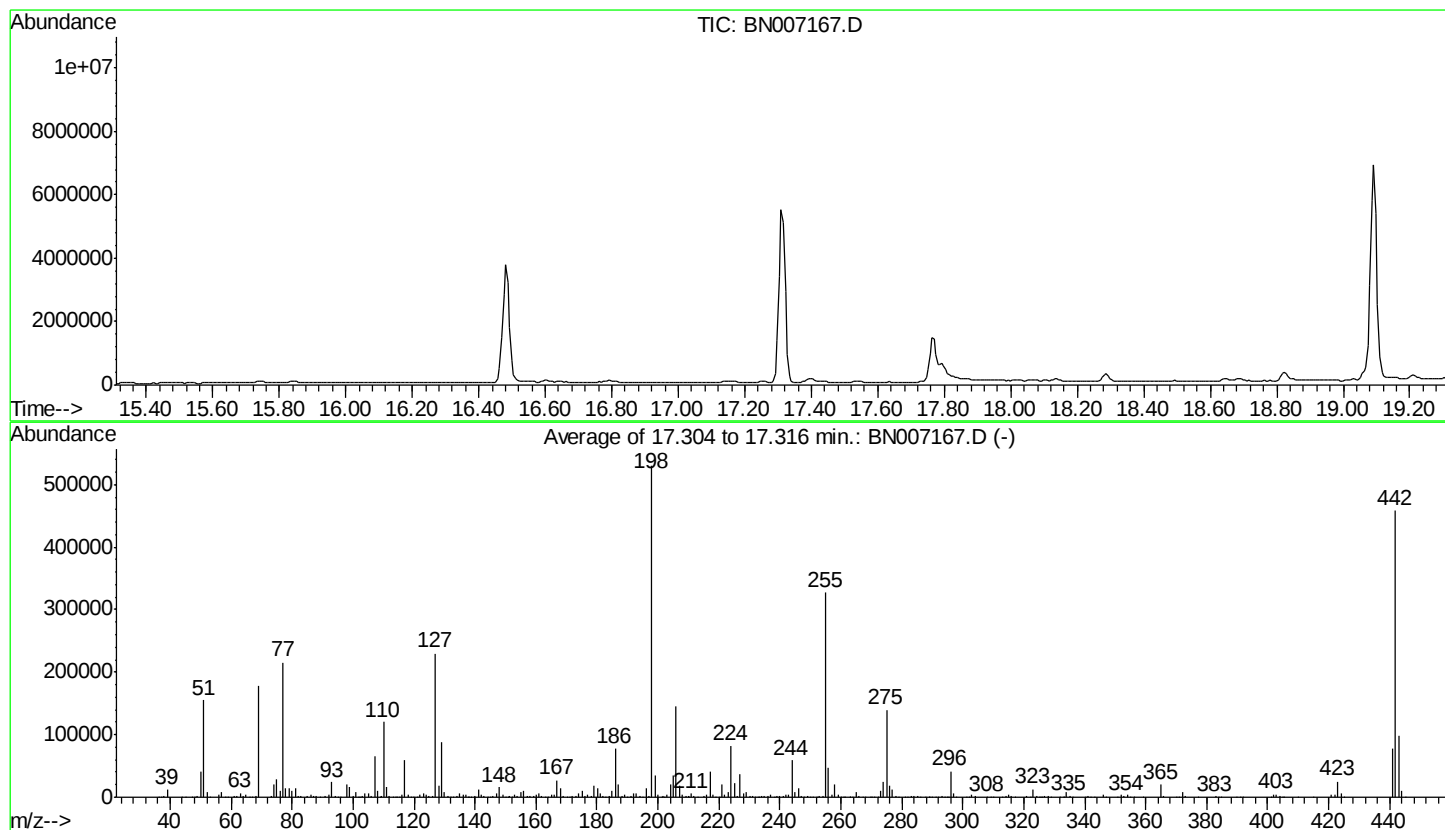

AutoFind: Scans 2434, 2435, 2436; Background Corrected with Scan 2427

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.3	155440	PASS
68	69	0.00	2	1.7	2954	PASS
69	198	0.00	100	33.5	177517	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	43.4	230172	PASS
197	198	0.00	2	0.4	2164	PASS
198	198	100	100	100.0	530304	PASS
199	198	5	9	6.7	35666	PASS
275	198	10	60	26.3	139664	PASS
365	198	1	100	3.7	19808	PASS
441	198	0.01	100	14.6	77301	PASS
442	198	50	100	86.4	458069	PASS
443	442	15	24	21.3	97672	PASS