

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081424\
 Data File : BN033376.D
 Acq On : 14 Aug 2024 10:19
 Operator : MA/JU
 Sample : PB162636BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK636

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081424.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN033376.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.158	8	12	25	rVB	71980	102157	1.15%	0.128%
2	3.540	73	77	95	rBV	955218	1499098	16.91%	1.880%
3	3.864	128	132	138	rVB	17386	23200	0.26%	0.029%
4	6.746	615	622	637	rBV	1158728	1756578	19.82%	2.203%
5	6.916	644	651	662	rVB	963733	1453367	16.40%	1.823%
6	7.105	676	683	692	rBV	1111053	1697837	19.15%	2.130%
7	7.569	754	762	770	rBV	996125	1511399	17.05%	1.896%
8	8.269	873	881	891	rBV	1446685	2191546	24.72%	2.749%
9	8.705	947	955	969	rBV	1104611	1790133	20.20%	2.246%
10	9.422	1070	1077	1089	rBV	765234	1237332	13.96%	1.552%
11	9.957	1160	1168	1180	rBV	1373001	2158065	24.35%	2.707%
12	10.334	1224	1232	1240	rBV	1451477	2350364	26.52%	2.948%
13	10.469	1246	1255	1265	rBV	1542527	2517931	28.41%	3.159%
14	11.934	1498	1504	1508	rBV2	24121	39914	0.45%	0.050%
15	13.628	1785	1792	1803	rBV	2819422	3859845	43.54%	4.842%
16	13.898	1829	1838	1846	rBV	2973126	4461083	50.33%	5.596%
17	14.204	1881	1890	1899	rBV	2322732	3443363	38.85%	4.319%
18	14.404	1918	1924	1943	rBV	1488713	2060772	23.25%	2.585%
19	14.634	1959	1963	1973	rVB10	6573	12479	0.14%	0.016%
20	15.204	2052	2060	2068	rBV	3978649	5640516	63.63%	7.076%
21	15.322	2073	2080	2091	rBV	1024147	1379862	15.57%	1.731%
22	15.451	2096	2102	2108	rVB4	18306	32032	0.36%	0.040%
23	15.992	2190	2194	2198	rVB3	10381	14823	0.17%	0.019%
24	16.739	2318	2321	2326	rVB2	7714	9969	0.11%	0.013%
25	16.957	2351	2358	2365	rBV	3095287	4306203	48.58%	5.402%
26	17.057	2368	2375	2385	rBV	4751550	6439456	72.65%	8.078%
27	17.886	2512	2516	2522	rBV6	24634	36656	0.41%	0.046%
28	18.922	2687	2692	2697	rVB	58559	76765	0.87%	0.096%
29	18.992	2699	2704	2709	rVB	51062	65691	0.74%	0.082%
30	19.181	2732	2736	2740	rBV6	22228	31412	0.35%	0.039%
31	19.357	2760	2766	2776	rBV2	5801823	7738765	87.30%	9.708%
32	21.192	3072	3078	3086	rBV	3686519	5108244	57.63%	6.408%
33	23.833	3517	3527	3540	rBV2	3903595	8864164	100.00%	11.119%
34	24.021	3550	3559	3574	rVB	2480780	5807331	65.51%	7.285%

Sum of corrected areas: 79718352

Instrument :

BNA_N

ClientSampleId :




SBLK636

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081424\
Data File : BN033376.D
Acq On : 14 Aug 2024 10:19
Operator : MA/JU
Sample : PB162636BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK636

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081424.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

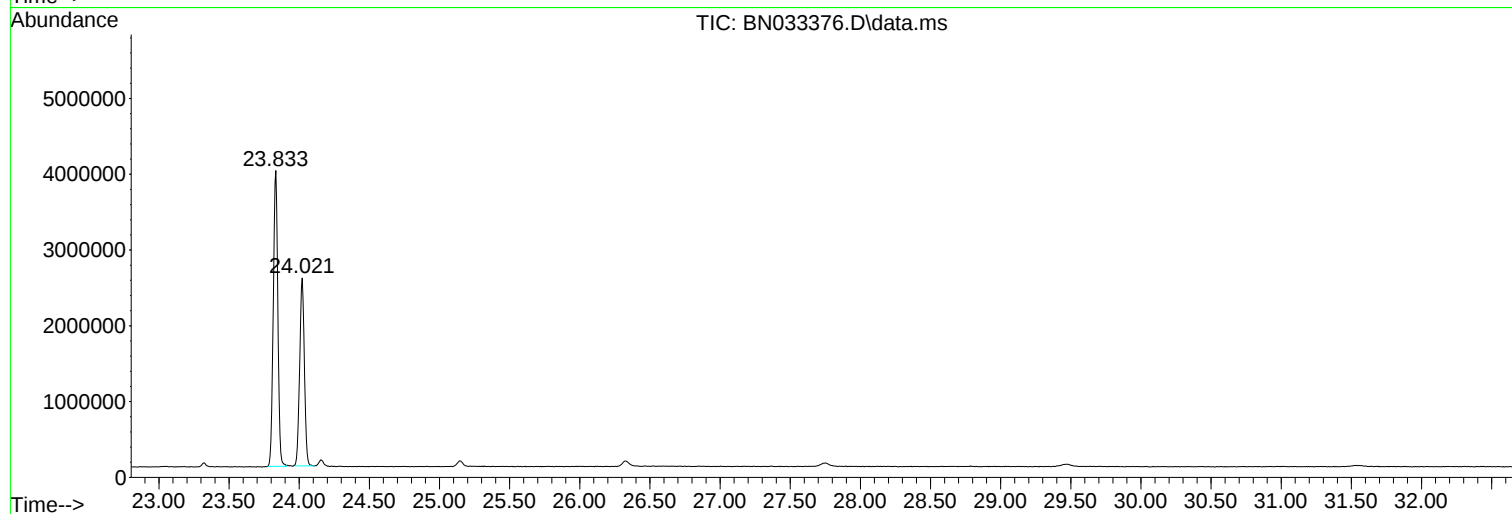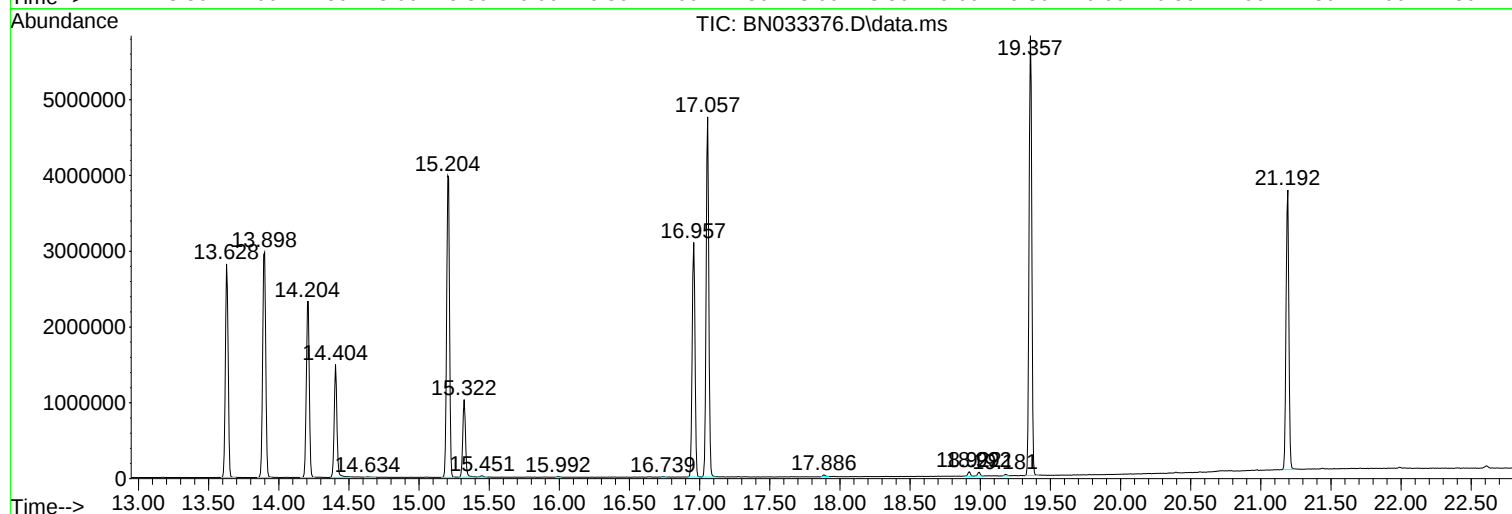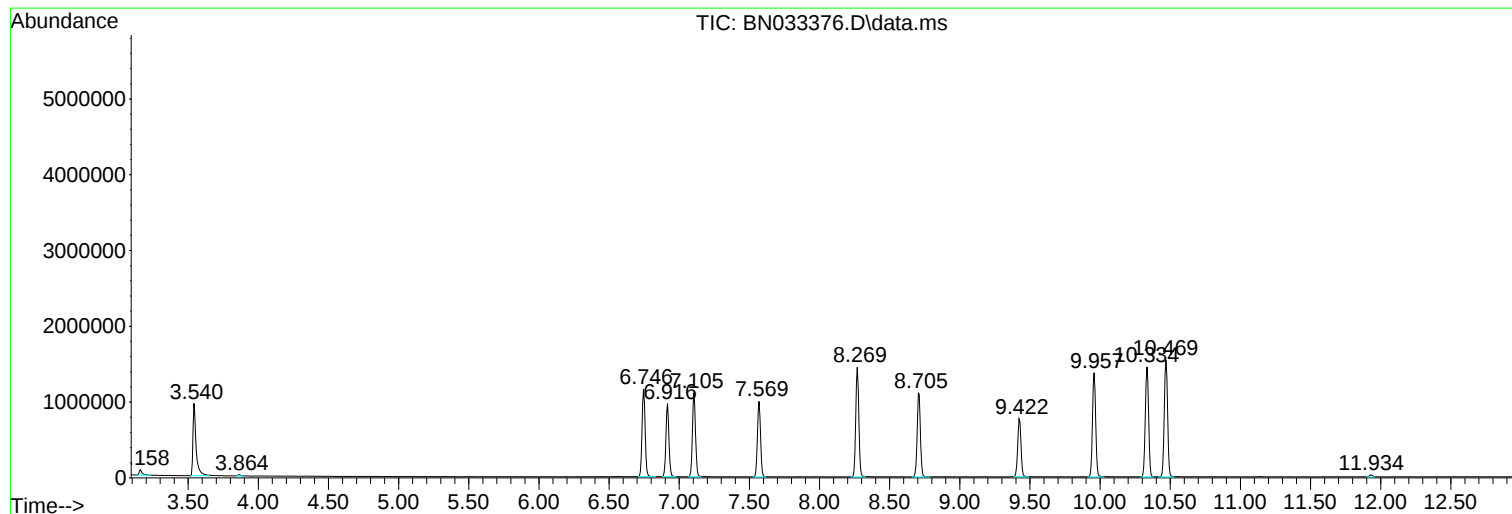

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081424\
Data File : BN033376.D
Acq On : 14 Aug 2024 10:19
Operator : MA/JU
Sample : PB162636BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK636

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081424.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081424\
Data File : BN033376.D
Acq On : 14 Aug 2024 10:19
Operator : MA/JU
Sample : PB162636BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK636

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081424.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc