

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081424\
 Data File : BN033387.D
 Acq On : 14 Aug 2024 18:34
 Operator : MA/JU
 Sample : PB162649BL
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK649

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081424.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN033387.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.158	25	29	42	rVB	73653	109075	1.29%	0.122%
2	3.540	90	94	113	rBV	1009873	1517653	17.97%	1.703%
3	3.863	145	149	152	rBV2	15132	17928	0.21%	0.020%
4	6.575	606	610	615	rVB6	6694	9639	0.11%	0.011%
5	6.751	632	640	648	rBV	1396579	2157315	25.54%	2.421%
6	6.916	662	668	677	rVB	1120321	1661394	19.67%	1.864%
7	7.104	693	700	708	rBV	1288458	2049046	24.26%	2.299%
8	7.569	772	779	790	rVB	1090201	1666539	19.73%	1.870%
9	8.275	887	899	908	rBV	1731648	2785252	32.97%	3.125%
10	8.710	965	973	980	rBV	1343249	2132343	25.24%	2.393%
11	9.422	1083	1094	1109	rBV	1012466	1684746	19.94%	1.890%
12	9.669	1131	1136	1141	rBV5	11207	17932	0.21%	0.020%
13	9.957	1176	1185	1194	rBV	1737262	2864757	33.91%	3.214%
14	10.334	1238	1249	1260	rBV	1641388	2746054	32.51%	3.081%
15	10.469	1264	1272	1282	rBV	1673929	2789903	33.03%	3.130%
16	11.145	1382	1387	1392	rBV6	11415	21082	0.25%	0.024%
17	11.934	1516	1521	1527	rVB2	32613	54283	0.64%	0.061%
18	13.175	1727	1732	1738	rBV4	7722	16042	0.19%	0.018%
19	13.633	1803	1810	1820	rBV	3029466	4273787	50.60%	4.795%
20	13.898	1848	1855	1863	rBV	3569811	5286615	62.59%	5.932%
21	14.210	1901	1908	1916	rBV	2687889	3881266	45.95%	4.355%
22	14.286	1916	1921	1927	rVB10	6908	12031	0.14%	0.013%
23	14.410	1935	1942	1958	rBV	1742952	2435560	28.83%	2.733%
24	15.210	2071	2078	2085	rBV	4676192	6503027	76.99%	7.297%
25	15.322	2090	2097	2111	rVV	1306163	1733312	20.52%	1.945%
26	15.445	2114	2118	2125	rVB3	20783	34794	0.41%	0.039%
27	15.998	2207	2212	2217	rVB3	15476	21891	0.26%	0.025%
28	16.639	2318	2321	2327	rVB6	8077	9867	0.12%	0.011%
29	16.745	2333	2339	2347	rBV3	9369	15696	0.19%	0.018%
30	16.957	2368	2375	2382	rBV	3389116	4634889	54.87%	5.201%
31	17.057	2385	2392	2404	rVV2	5214908	7067825	83.67%	7.931%
32	17.198	2414	2416	2424	rVB8	5114	9223	0.11%	0.010%
33	17.339	2436	2440	2447	rVB7	13272	24016	0.28%	0.027%
34	17.657	2490	2494	2501	rVB5	6053	12864	0.15%	0.014%
35	17.886	2529	2533	2540	rBV3	30000	52059	0.62%	0.058%
36	18.180	2578	2583	2589	rBV4	35110	56415	0.67%	0.063%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081424\
Data File : BN033387.D
Acq On : 14 Aug 2024 18:34
Operator : MA/JU
Sample : PB162649BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK649

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081424.MA.M
Title : SVOA CALIBRATION

37	18.327	2606	2608	2615	rBV8	6181	10776	0.13%	0.012%
38	18.763	2679	2682	2686	rVB5	6744	8765	0.10%	0.010%
39	18.921	2704	2709	2715	rBV2	66585	89930	1.06%	0.101%
40	18.992	2717	2721	2726	rVV	68419	87616	1.04%	0.098%
41	19.180	2750	2753	2757	rBV5	20462	25091	0.30%	0.028%
42	19.363	2777	2784	2789	rBV	6276617	8447018	100.00%	9.478%
43	19.421	2789	2794	2803	rVB	181686	280048	3.32%	0.314%
44	21.192	3089	3095	3107	rBV	3907303	5335266	63.16%	5.986%
45	23.315	3452	3456	3466	rVB2	93465	187940	2.22%	0.211%
46	23.833	3534	3544	3557	rBV2	3634980	8411122	99.58%	9.438%
47	24.021	3567	3576	3587	rVB2	2227874	5137231	60.82%	5.764%
48	24.151	3593	3598	3607	rVB2	158454	333472	3.95%	0.374%
49	25.139	3761	3766	3779	rVB3	154609	401410	4.75%	0.450%




Sum of corrected areas: 89121805

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081424\
Data File : BN033387.D
Acq On : 14 Aug 2024 18:34
Operator : MA/JU
Sample : PB162649BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK649

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081424.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

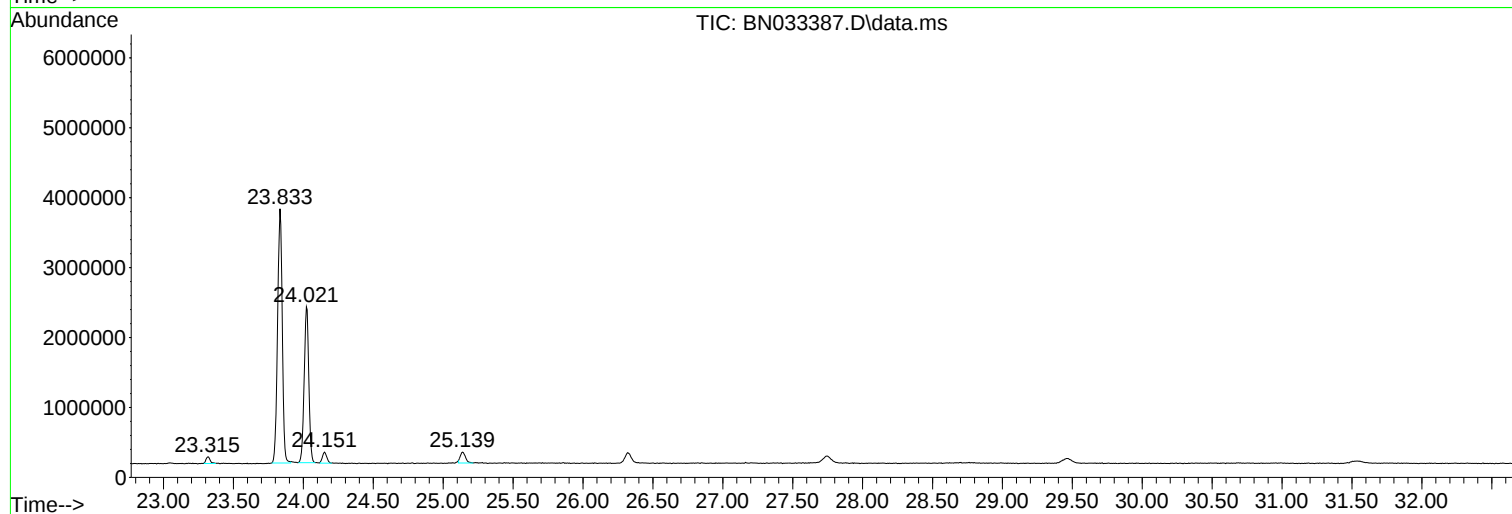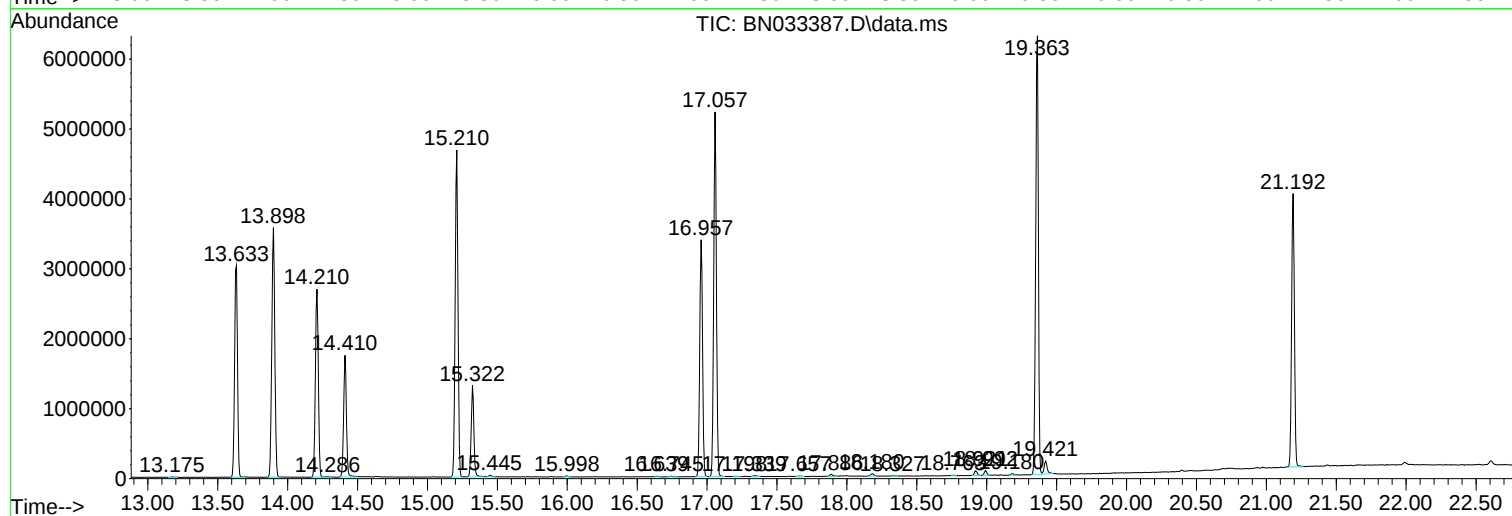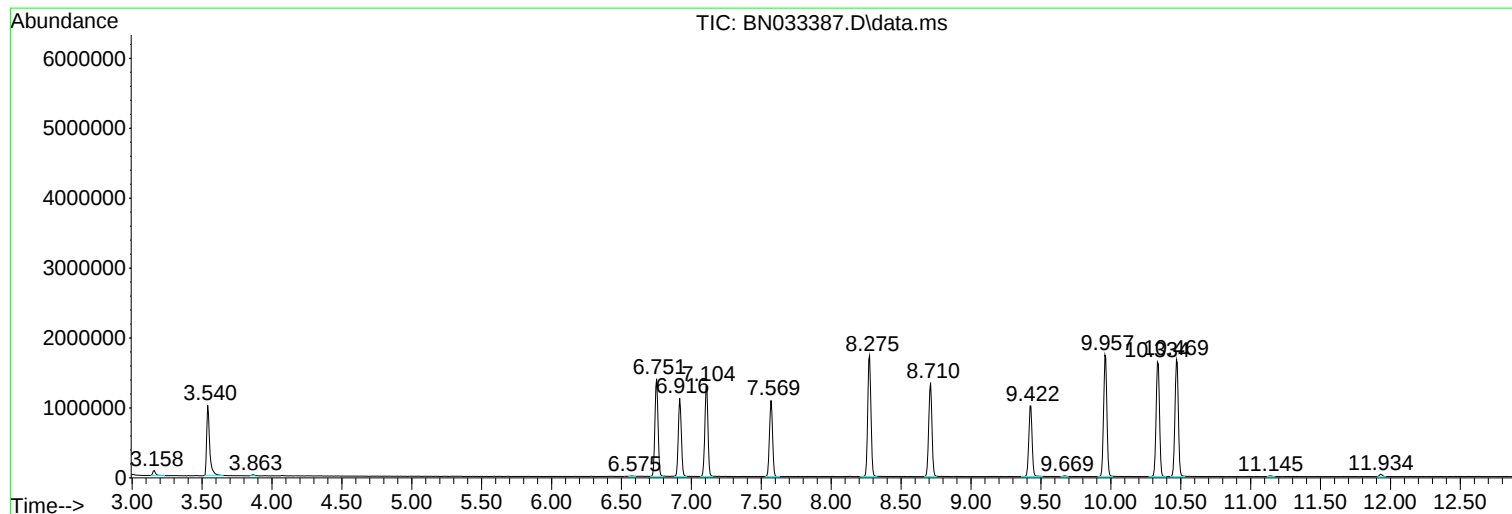

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081424\
Data File : BN033387.D
Acq On : 14 Aug 2024 18:34
Operator : MA/JU
Sample : PB162649BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK649

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081424.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081424\
Data File : BN033387.D
Acq On : 14 Aug 2024 18:34
Operator : MA/JU
Sample : PB162649BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK649

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081424.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc