

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081424\
 Data File : BN033389.D
 Acq On : 14 Aug 2024 19:52
 Operator : MA/JU
 Sample : P3481-03
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E0AE3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081424.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN033389.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.081	14	16	22	rVB8	8316	11731	0.20%	0.022%
2	3.158	25	29	40	rVB	32098	53363	0.92%	0.099%
3	3.411	68	72	81	rBV	31088	48139	0.83%	0.089%
4	3.546	90	95	110	rBV	291205	462109	7.92%	0.854%
5	3.864	145	149	154	rBV	13629	20463	0.35%	0.038%
6	5.340	395	400	403	rVB6	4138	6285	0.11%	0.012%
7	5.699	457	461	469	rVB2	12009	17091	0.29%	0.032%
8	6.575	607	610	614	rBV4	4651	7304	0.13%	0.014%
9	6.746	632	639	651	rBV	599740	951793	16.32%	1.760%
10	6.875	655	661	662	rBV4	7669	11399	0.20%	0.021%
11	6.917	662	668	679	rVB	477427	732991	12.57%	1.355%
12	7.105	693	700	709	rBV	600215	924864	15.86%	1.710%
13	7.187	710	714	720	rVV	18436	26311	0.45%	0.049%
14	7.569	771	779	787	rVB	1275385	1937410	33.23%	3.582%
15	7.646	787	792	800	rBV5	12132	21630	0.37%	0.040%
16	8.269	890	898	906	rBV	792353	1224933	21.01%	2.265%
17	8.705	964	972	980	rBV	549533	898049	15.40%	1.661%
18	9.187	1051	1054	1059	rVB7	3835	5881	0.10%	0.011%
19	9.287	1066	1071	1080	rVB	55003	81827	1.40%	0.151%
20	9.422	1087	1094	1102	rBV	408857	647912	11.11%	1.198%
21	9.663	1130	1135	1140	rBV9	4585	8882	0.15%	0.016%
22	9.958	1178	1185	1197	rBV	773001	1240875	21.28%	2.294%
23	10.334	1241	1249	1257	rBV	1913717	3146206	53.95%	5.817%
24	10.469	1265	1272	1283	rBV	428116	692960	11.88%	1.281%
25	10.893	1339	1344	1350	rVB	30249	45732	0.78%	0.085%
26	11.081	1367	1376	1383	rBV	175437	298393	5.12%	0.552%
27	11.134	1383	1385	1390	rVB5	5578	9214	0.16%	0.017%
28	11.928	1513	1520	1526	rBV2	17687	29580	0.51%	0.055%
29	12.569	1625	1629	1634	rBV7	4159	7281	0.12%	0.013%
30	13.628	1802	1809	1818	rBV	1395221	1848305	31.70%	3.418%
31	13.899	1848	1855	1863	rBV	1546408	2293617	39.33%	4.241%
32	14.210	1901	1908	1915	rBV	3079538	4421171	75.82%	8.175%
33	14.404	1935	1941	1946	rBV	535843	773357	13.26%	1.430%
34	14.446	1946	1948	1949	rVV2	66494	67353	1.16%	0.125%
35	14.463	1949	1951	1962	rVB	71923	89720	1.54%	0.166%
36	14.640	1977	1981	1986	rBV7	5988	12471	0.21%	0.023%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081424\
 Data File : BN033389.D
 Acq On : 14 Aug 2024 19:52
 Operator : MA/JU
 Sample : P3481-03
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E0AE3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081424.MA.M
 Title : SVOA CALIBRATION

37	15.046	2047	2050	2055	rVB4	8212	10644	0.18%	0.020%
38	15.210	2071	2078	2084	rBV	1953402	2823425	48.42%	5.221%
39	15.322	2092	2097	2104	rBV	318172	439090	7.53%	0.812%
40	15.446	2115	2118	2123	rVB6	11465	15316	0.26%	0.028%
41	15.787	2175	2176	2181	rVB4	5966	8123	0.14%	0.015%
42	15.975	2205	2208	2210	rBV4	6442	7717	0.13%	0.014%
43	16.393	2276	2279	2283	rVB6	6101	7984	0.14%	0.015%
44	16.551	2303	2306	2312	rBV6	6660	9145	0.16%	0.017%
45	16.722	2330	2335	2336	rBV5	6940	10077	0.17%	0.019%
46	16.745	2336	2339	2342	rVV3	6824	9246	0.16%	0.017%
47	16.957	2368	2375	2385	rBV	3916033	5312280	91.10%	9.823%
48	17.057	2385	2392	2403	rVB	2282670	3067786	52.61%	5.672%
49	17.163	2406	2410	2415	rVB6	14073	18730	0.32%	0.035%
50	17.345	2437	2441	2450	rVB3	22058	37605	0.64%	0.070%
51	17.675	2495	2497	2501	rVB3	11180	12217	0.21%	0.023%
52	17.757	2508	2511	2518	rBV8	6826	12735	0.22%	0.024%
53	17.887	2529	2533	2541	rBV	150734	220732	3.79%	0.408%
54	18.181	2579	2583	2589	rVB6	16450	24605	0.42%	0.045%
55	18.769	2679	2683	2688	rBV6	10530	17865	0.31%	0.033%
56	18.922	2706	2709	2714	rVB3	31976	39480	0.68%	0.073%
57	18.992	2717	2721	2724	rBV	36842	53284	0.91%	0.099%
58	19.028	2724	2727	2730	rVV3	22181	29307	0.50%	0.054%
59	19.057	2730	2732	2737	rVB5	10641	16285	0.28%	0.030%
60	19.181	2749	2753	2758	rBV2	64407	87453	1.50%	0.162%
61	19.357	2777	2783	2789	rBV	2730773	3672196	62.98%	6.790%
62	19.422	2789	2794	2798	rVV	235485	311552	5.34%	0.576%
63	20.922	3046	3049	3055	rBV2	113343	153631	2.63%	0.284%
64	21.192	3089	3095	3103	rBV	4317066	5831171	100.00%	10.782%
65	23.827	3535	3543	3556	rVB	1395537	3220131	55.22%	5.954%
66	24.027	3568	3577	3591	rVB	2334859	5526067	94.77%	10.218%




Sum of corrected areas: 54082481

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081424\
Data File : BN033389.D
Acq On : 14 Aug 2024 19:52
Operator : MA/JU
Sample : P3481-03
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E0AE3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081424.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

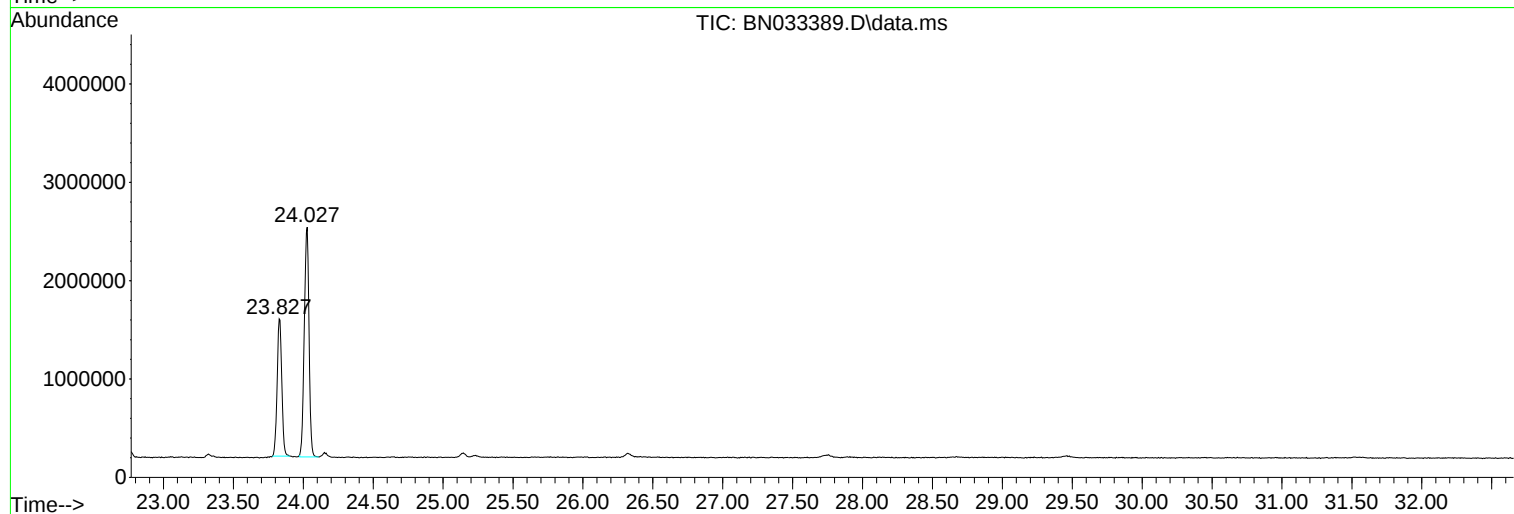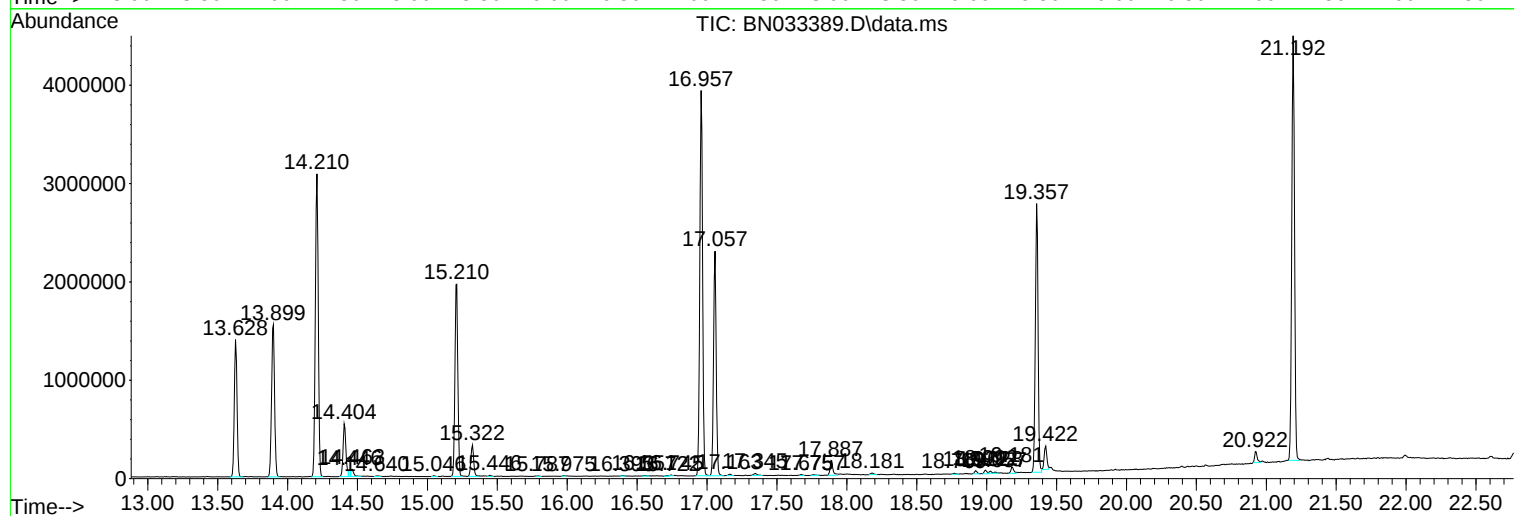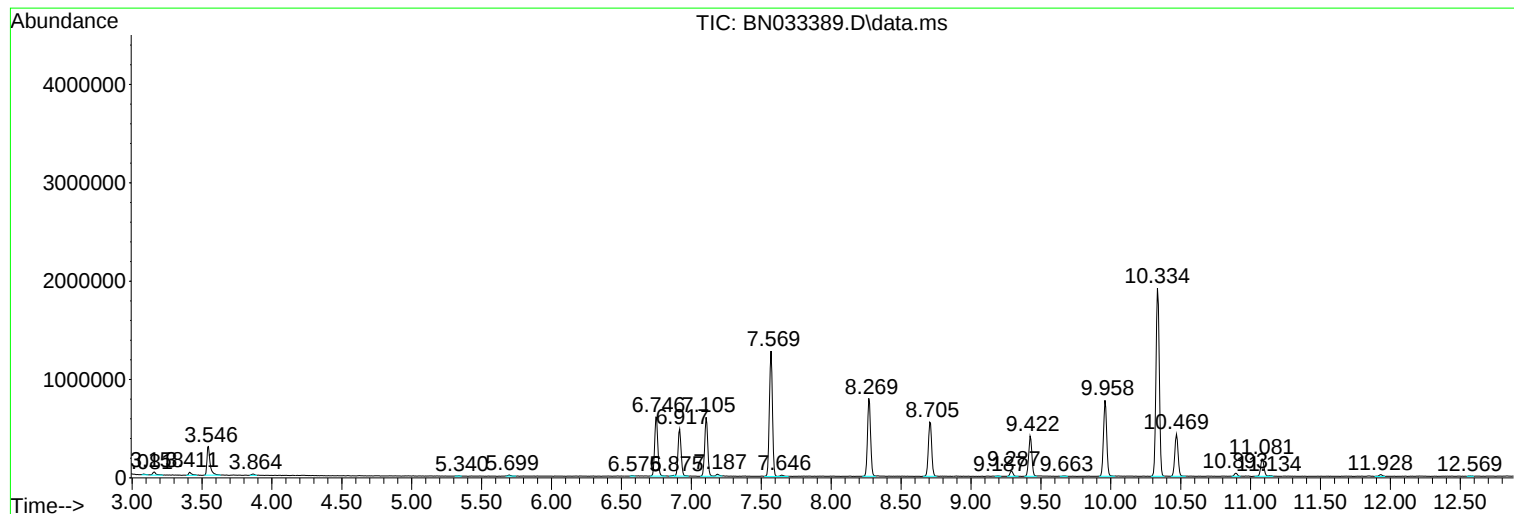

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081424\
Data File : BN033389.D
Acq On : 14 Aug 2024 19:52
Operator : MA/JU
Sample : P3481-03
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E0AE3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081424.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081424\
Data File : BN033389.D
Acq On : 14 Aug 2024 19:52
Operator : MA/JU
Sample : P3481-03
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E0AE3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081424.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc