

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081424\
 Data File : BN033390.D
 Acq On : 14 Aug 2024 20:32
 Operator : MA/JU
 Sample : P3481-05
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E0AD7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081424.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN033390.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.081	13	16	19	rVB2	10304	11708	0.20%	0.016%
2	3.158	25	29	36	rBV	55979	74513	1.26%	0.100%
3	3.411	68	72	83	rBV	50485	74791	1.26%	0.100%
4	3.540	90	94	110	rBV	504924	768500	12.97%	1.027%
5	3.864	145	149	154	rVB	18164	25145	0.42%	0.034%
6	4.328	223	228	231	rBV6	4246	7385	0.12%	0.010%
7	5.322	394	397	402	rBV3	8126	12496	0.21%	0.017%
8	5.693	454	460	468	rBV	19728	33685	0.57%	0.045%
9	6.169	536	541	542	rBV5	5669	7774	0.13%	0.010%
10	6.575	605	610	612	rBV3	7191	9213	0.16%	0.012%
11	6.752	628	640	648	rBV	1028774	1641539	27.71%	2.194%
12	6.916	661	668	680	rVB	853261	1266066	21.37%	1.692%
13	7.105	693	700	709	rBV	1045040	1602311	27.05%	2.141%
14	7.187	709	714	718	rBV	36626	55867	0.94%	0.075%
15	7.569	772	779	786	rBV	1461637	2204189	37.21%	2.946%
16	7.646	786	792	797	rVB2	18100	27074	0.46%	0.036%
17	7.805	815	819	824	rBV6	4158	8927	0.15%	0.012%
18	8.269	890	898	906	rBV	1316941	2071727	34.97%	2.769%
19	8.710	965	973	982	rBV	971375	1566535	26.45%	2.094%
20	8.811	986	990	993	rVV3	8057	13016	0.22%	0.017%
21	8.893	999	1004	1008	rBV8	6125	11115	0.19%	0.015%
22	9.293	1066	1072	1077	rBV	86039	130778	2.21%	0.175%
23	9.422	1085	1094	1104	rBV	741941	1183831	19.98%	1.582%
24	9.663	1132	1135	1141	rVB4	10595	15213	0.26%	0.020%
25	9.834	1160	1164	1167	rBV6	6998	9204	0.16%	0.012%
26	9.958	1177	1185	1197	rBV	1276550	2075749	35.04%	2.774%
27	10.334	1241	1249	1257	rBV	2093388	3465849	58.51%	4.632%
28	10.469	1265	1272	1279	rBV	740008	1198242	20.23%	1.601%
29	10.534	1279	1283	1287	rVB5	8039	13065	0.22%	0.017%
30	10.810	1326	1330	1333	rVB6	6736	7943	0.13%	0.011%
31	10.893	1340	1344	1351	rVB	54220	82365	1.39%	0.110%
32	10.975	1354	1358	1363	rVB7	4614	7429	0.13%	0.010%
33	11.081	1369	1376	1383	rBV	311795	518741	8.76%	0.693%
34	11.140	1383	1386	1393	rVB6	13272	21707	0.37%	0.029%
35	11.393	1421	1429	1430	rBV5	7097	16085	0.27%	0.021%
36	11.799	1491	1498	1504	rBV5	13549	26716	0.45%	0.036%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081424\
 Data File : BN033390.D
 Acq On : 14 Aug 2024 20:32
 Operator : MA/JU
 Sample : P3481-05
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E0AD7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081424.MA.M
 Title : SVOA CALIBRATION

37	11.852	1504	1507	1511	rVV3	6707	8393	0.14%	0.011%
38	11.934	1514	1521	1527	rVV	28753	48118	0.81%	0.064%
39	12.487	1611	1615	1618	rBV6	4752	8010	0.14%	0.011%
40	12.569	1626	1629	1634	rVB7	5393	8308	0.14%	0.011%
41	12.634	1634	1640	1645	rBV9	4841	8706	0.15%	0.012%
42	13.004	1696	1703	1706	rBV9	6941	15397	0.26%	0.021%
43	13.063	1708	1713	1719	rVV	16644	25203	0.43%	0.034%
44	13.134	1721	1725	1729	rVV6	5145	9429	0.16%	0.013%
45	13.210	1735	1738	1744	rVB5	9184	13964	0.24%	0.019%
46	13.422	1771	1774	1779	rBV5	6178	9310	0.16%	0.012%
47	13.628	1803	1809	1816	rBV	2210720	2996449	50.58%	4.005%
48	13.734	1823	1827	1832	rVB6	9355	13320	0.22%	0.018%
49	13.898	1848	1855	1862	rBV	2477370	3749621	63.30%	5.011%
50	14.151	1895	1898	1901	rBV2	17534	20863	0.35%	0.028%
51	14.210	1901	1908	1915	rVB	3364602	4775920	80.63%	6.383%
52	14.410	1934	1942	1946	rBV	840393	1193575	20.15%	1.595%
53	14.446	1946	1948	1949	rBV2	27493	26797	0.45%	0.036%
54	14.640	1977	1981	1982	rBV4	7809	9263	0.16%	0.012%
55	14.740	1993	1998	2001	rBV4	8402	13609	0.23%	0.018%
56	15.051	2045	2051	2055	rBV8	7453	13788	0.23%	0.018%
57	15.110	2057	2061	2066	rVB2	17908	21809	0.37%	0.029%
58	15.204	2071	2077	2087	rBV	3143808	4579169	77.30%	6.120%
59	15.322	2091	2097	2109	rBV	530941	724263	12.23%	0.968%
60	15.445	2115	2118	2124	rVB	15854	23077	0.39%	0.031%
61	15.516	2127	2130	2136	rVB6	10003	16157	0.27%	0.022%
62	15.675	2152	2157	2161	rBV8	6833	11767	0.20%	0.016%
63	15.792	2171	2177	2180	rBV8	7641	11569	0.20%	0.015%
64	15.910	2194	2197	2202	rVB2	18518	24964	0.42%	0.033%
65	15.975	2204	2208	2210	rVV	24305	33268	0.56%	0.044%
66	15.998	2210	2212	2219	rVB4	23346	32501	0.55%	0.043%
67	16.398	2275	2280	2283	rBV5	11398	16800	0.28%	0.022%
68	16.481	2290	2294	2298	rBV6	5968	10443	0.18%	0.014%
69	16.551	2303	2306	2310	rBV6	7294	11237	0.19%	0.015%
70	16.769	2340	2343	2348	rVB3	14301	16083	0.27%	0.021%
71	16.957	2367	2375	2382	rBV	3962466	5600942	94.55%	7.485%
72	17.057	2385	2392	2404	rVV2	3510910	4829592	81.53%	6.455%
73	17.163	2406	2410	2415	rVB6	24966	32481	0.55%	0.043%
74	17.345	2436	2441	2452	rVV	100318	188645	3.18%	0.252%
75	17.504	2465	2468	2474	rBV3	13260	16280	0.27%	0.022%
76	17.675	2494	2497	2501	rVB3	14760	18970	0.32%	0.025%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081424\
 Data File : BN033390.D
 Acq On : 14 Aug 2024 20:32
 Operator : MA/JU
 Sample : P3481-05
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E0AD7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081424.MA.M
 Title : SVOA CALIBRATION

77	17.763	2507	2512	2517	rBV9	14827	28754	0.49%	0.038%
78	17.892	2528	2534	2542	rBV	344864	502352	8.48%	0.671%
79	18.186	2579	2584	2590	rBV6	19596	45421	0.77%	0.061%
80	18.334	2607	2609	2611	rBV3	8598	7576	0.13%	0.010%
81	18.357	2611	2613	2620	rVB7	13928	21606	0.36%	0.029%
82	18.763	2679	2682	2687	rVB7	13025	20080	0.34%	0.027%
83	18.845	2692	2696	2704	rBV5	14808	24596	0.42%	0.033%
84	18.922	2705	2709	2713	rVB3	51957	67332	1.14%	0.090%
85	18.992	2716	2721	2724	rBV	55407	77642	1.31%	0.104%
86	19.033	2724	2728	2730	rBV4	34163	41108	0.69%	0.055%
87	19.063	2730	2733	2738	rVB6	24705	37713	0.64%	0.050%
88	19.181	2749	2753	2759	rBV	138141	186878	3.15%	0.250%
89	19.357	2777	2783	2789	rBV	4308260	5712730	96.44%	7.635%
90	19.422	2789	2794	2798	rVV	368805	551988	9.32%	0.738%
91	19.457	2798	2800	2807	rVB	90145	117579	1.98%	0.157%
92	19.963	2883	2886	2890	rVB3	37644	37213	0.63%	0.050%
93	20.933	3045	3051	3062	rBV2	545553	1021323	17.24%	1.365%
94	21.192	3089	3095	3102	rBV	4170317	5923621	100.00%	7.917%
95	21.292	3109	3112	3116	rBV5	57085	72227	1.22%	0.097%
96	21.986	3225	3230	3242	rVB	318793	523255	8.83%	0.699%
97	22.769	3359	3363	3367	rBV	98331	142772	2.41%	0.191%
98	23.316	3452	3456	3459	rBV2	77826	136031	2.30%	0.182%
99	23.827	3534	3543	3555	rVB	2082323	4718173	79.65%	6.306%
100	24.021	3567	3576	3589	rVB	2315270	5352147	90.35%	7.153%




Sum of corrected areas: 74824670

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081424\
Data File : BN033390.D
Acq On : 14 Aug 2024 20:32
Operator : MA/JU
Sample : P3481-05
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E0AD7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081424.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

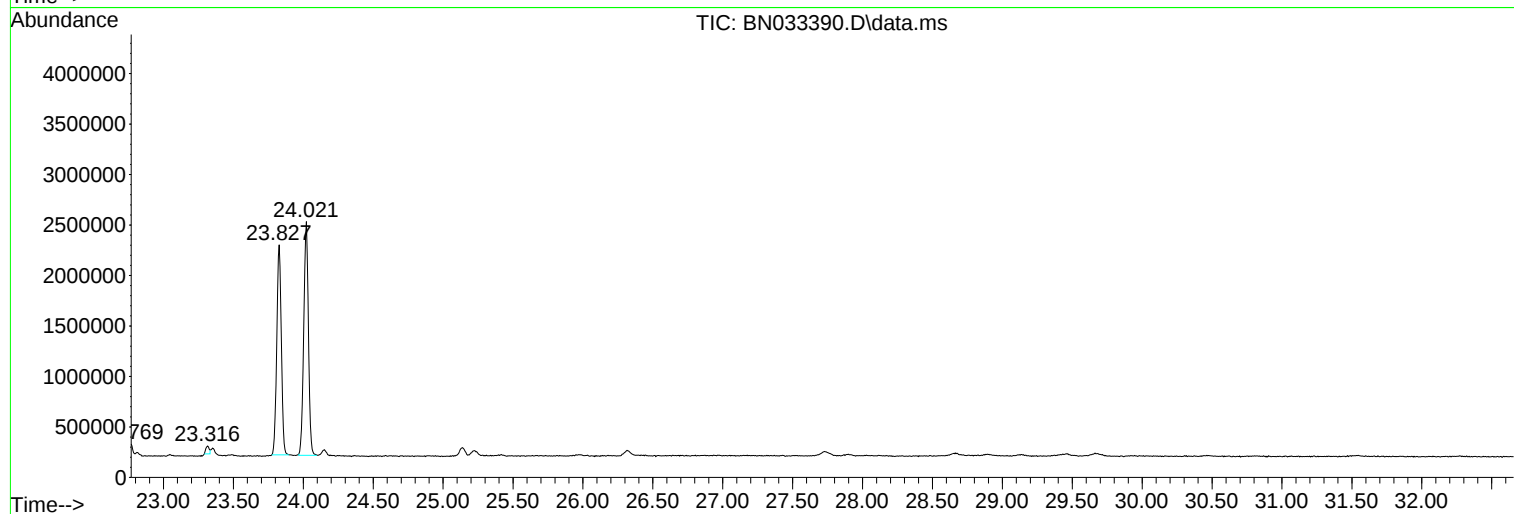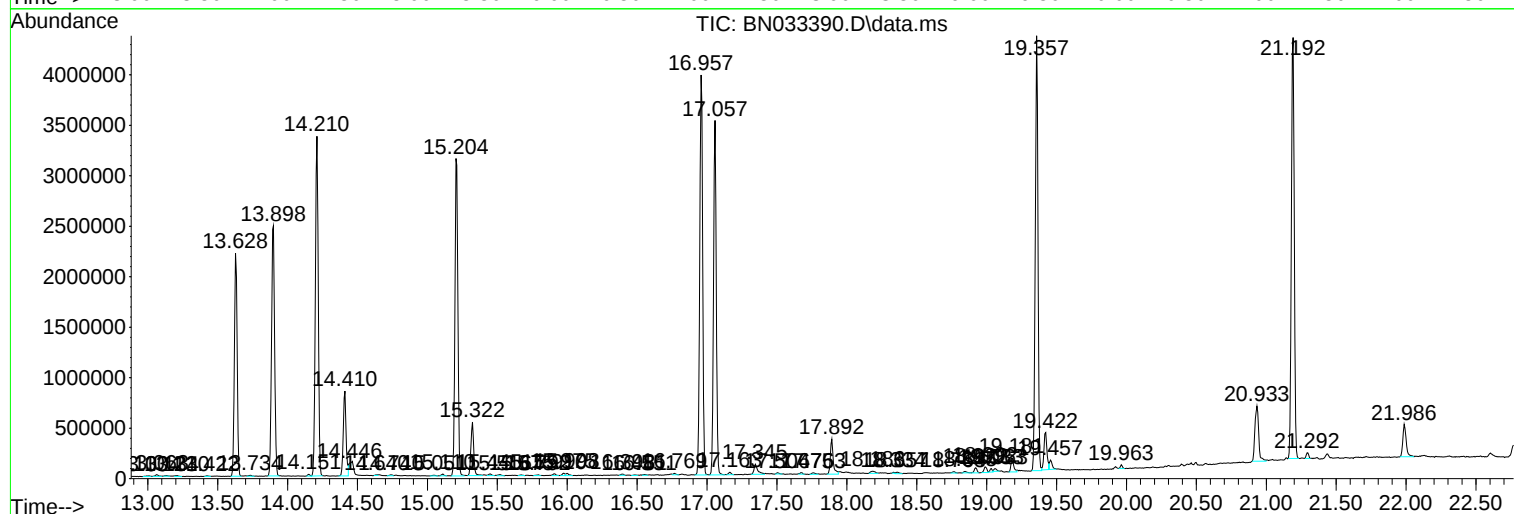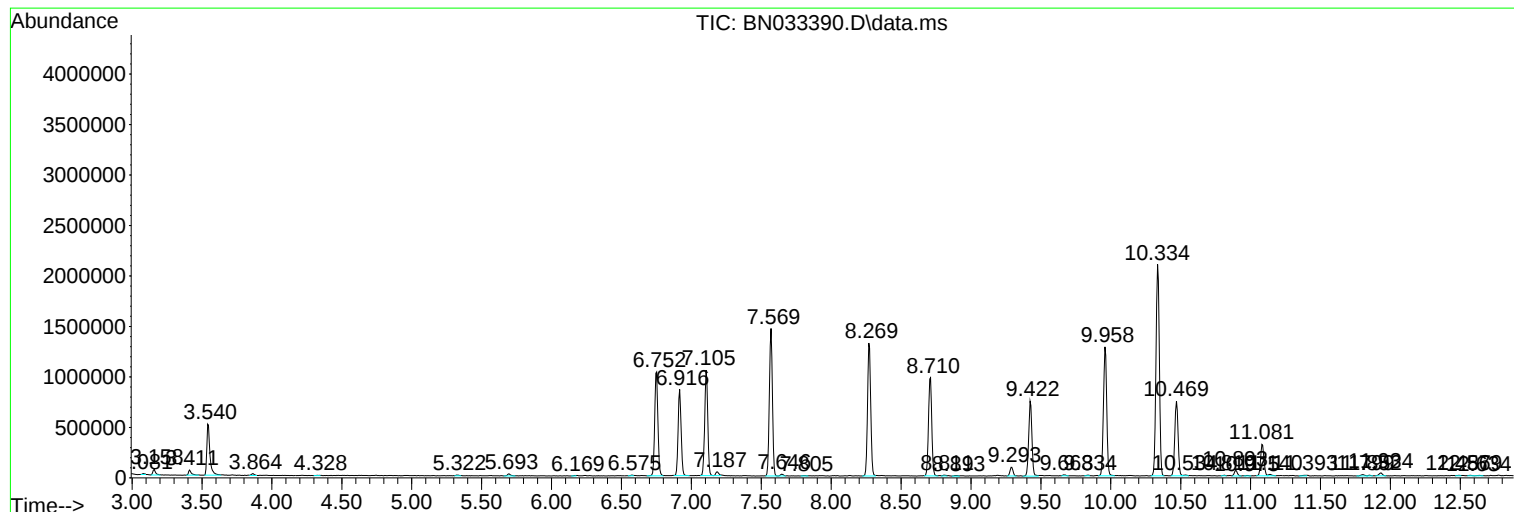

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081424\
Data File : BN033390.D
Acq On : 14 Aug 2024 20:32
Operator : MA/JU
Sample : P3481-05
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E0AD7










Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081424.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 1-Phenoxypropan-2-ol Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
11.081	2.99 ng/ul	518741	Naphthalene-d8	10.334

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	1-Phenoxypropan-2-ol			152	C9H12O2	000770-35-4	96
2	1-Phenoxypropan-2-ol			152	C9H12O2	000770-35-4	96
3	1-Phenoxypropan-2-ol			152	C9H12O2	000770-35-4	94
4	1-Phenoxypropan-2-ol			152	C9H12O2	000770-35-4	94
5	1-Propanol, 3-phenoxy-			152	C9H12O2	006180-61-6	87

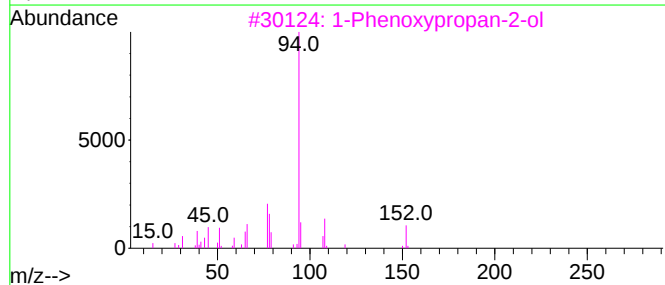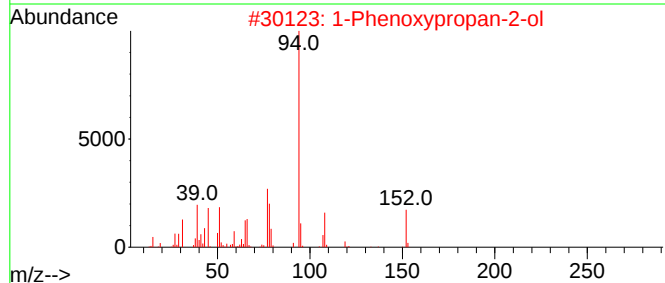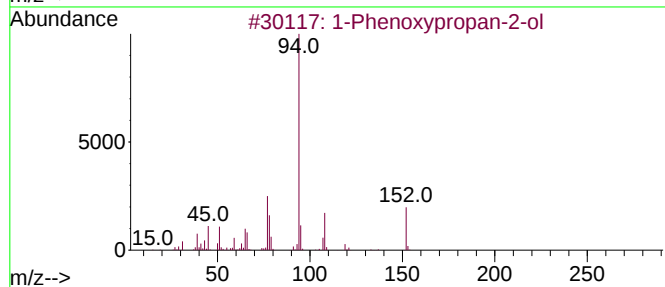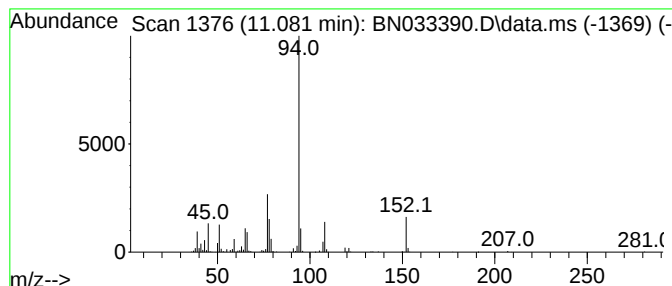

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081424\
Data File : BN033390.D
Acq On : 14 Aug 2024 20:32
Operator : MA/JU
Sample : P3481-05
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E0AD7










Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081424.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 (DEL) Alkane: Straight-Chai... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
20.933	3.45 ng/ul	1021320	Chrysene-d12	21.192

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Tetratetracontane	619	C44H90	007098-22-8	91
2			Sulfurous acid, butyl tetradecyl...	334	C18H38O3S	1010309-18-1	91
3			Heptadecane	240	C17H36	000629-78-7	90
4			Carbonic acid, tetradecyl vinyl ...	284	C17H32O3	1000382-54-5	87
5			Octacosane	394	C28H58	000630-02-4	83

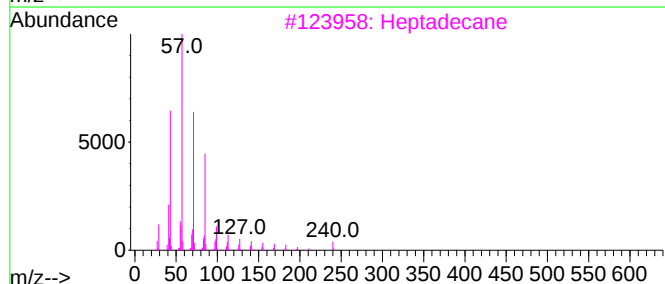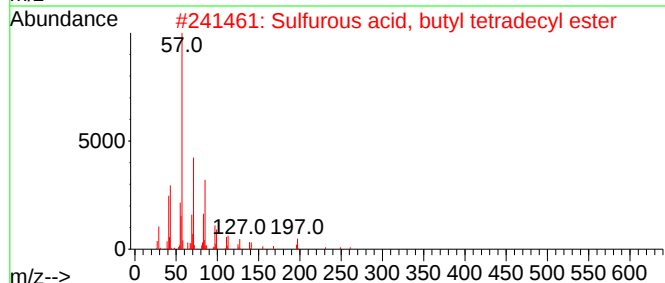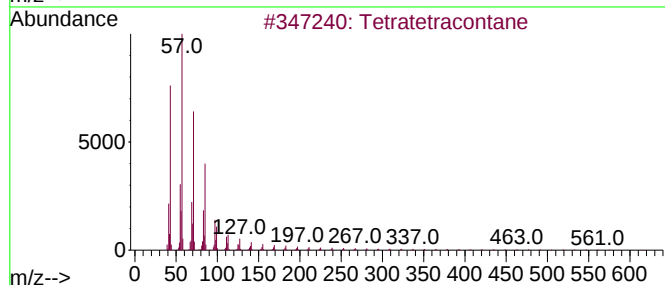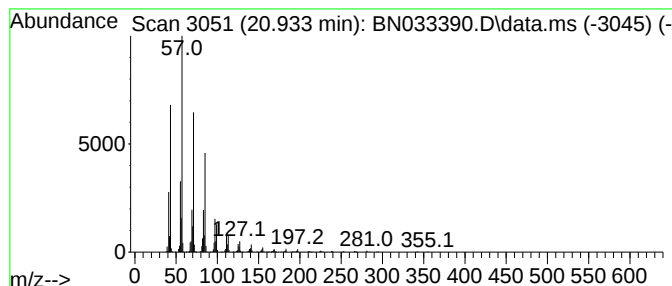

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN081424\
Data File : BN033390.D
Acq On : 14 Aug 2024 20:32
Operator : MA/JU
Sample : P3481-05
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E0AD7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN081424.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
1-Phenoxypropan...	11.081	3.0	ng/u1	518741	2	10.334	3465850	20.0
(DEL) Alkane: S...	20.933	3.5	ng/u1	1021320	5	21.192	5923620	20.0